


Magnetic field, magnetometer on power supply, RED: original, BLUE: new

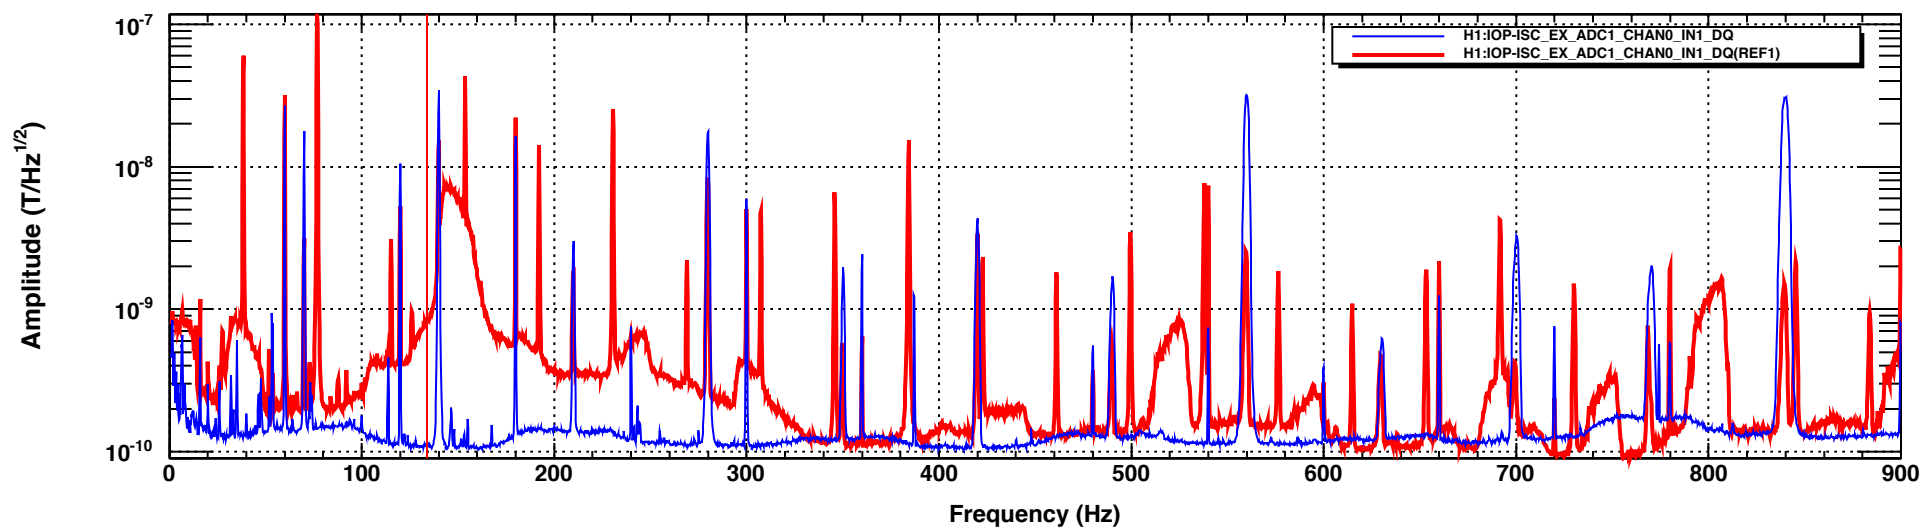


*T0=18/04/2015 16:23:43

Avg=1000

BW=0.374999

Coherence between magnetometer channel and channel terminated at AA chasis, RED original supply, BLUE: new, high only at 60 Hz harmonics

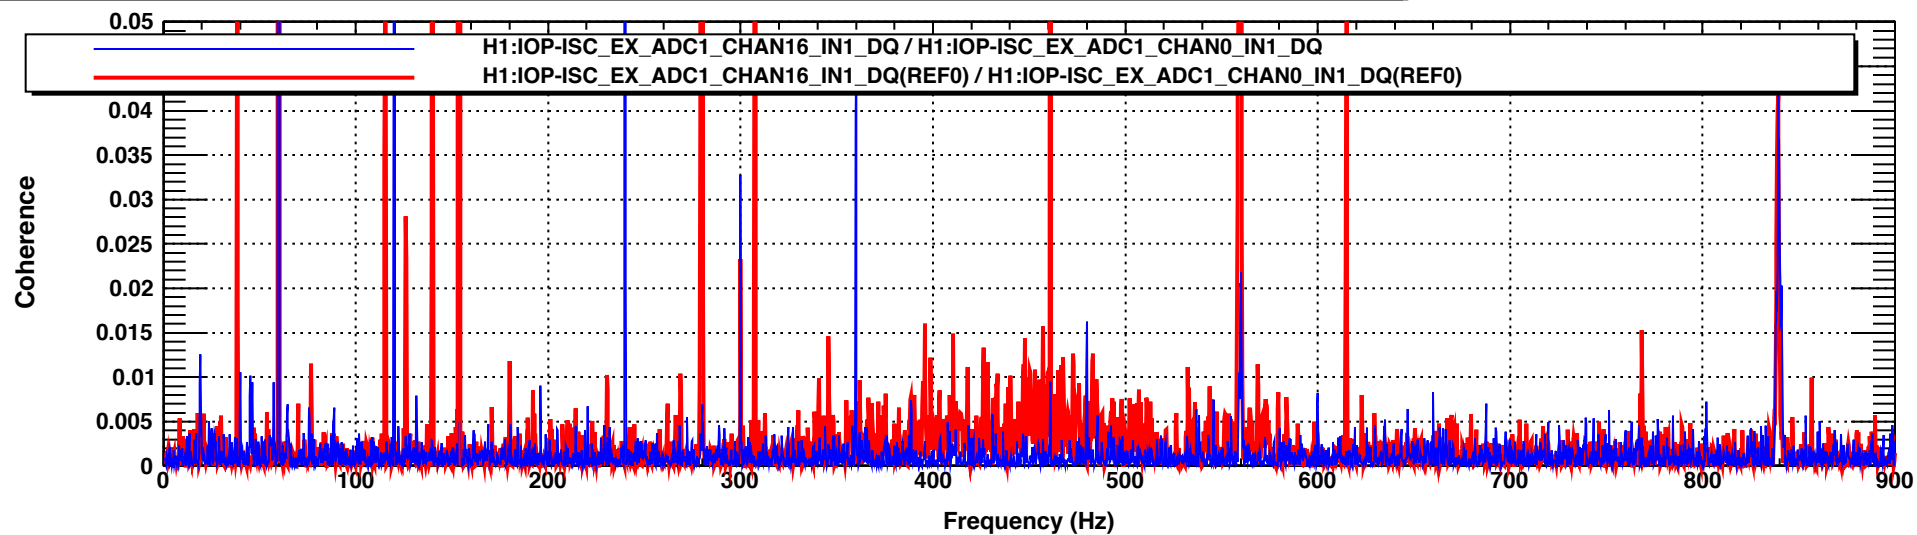

*T0=18/04/2015 16:23:43

Avg=1000

BW=0.374999