


DARM: with and without Calibration lines

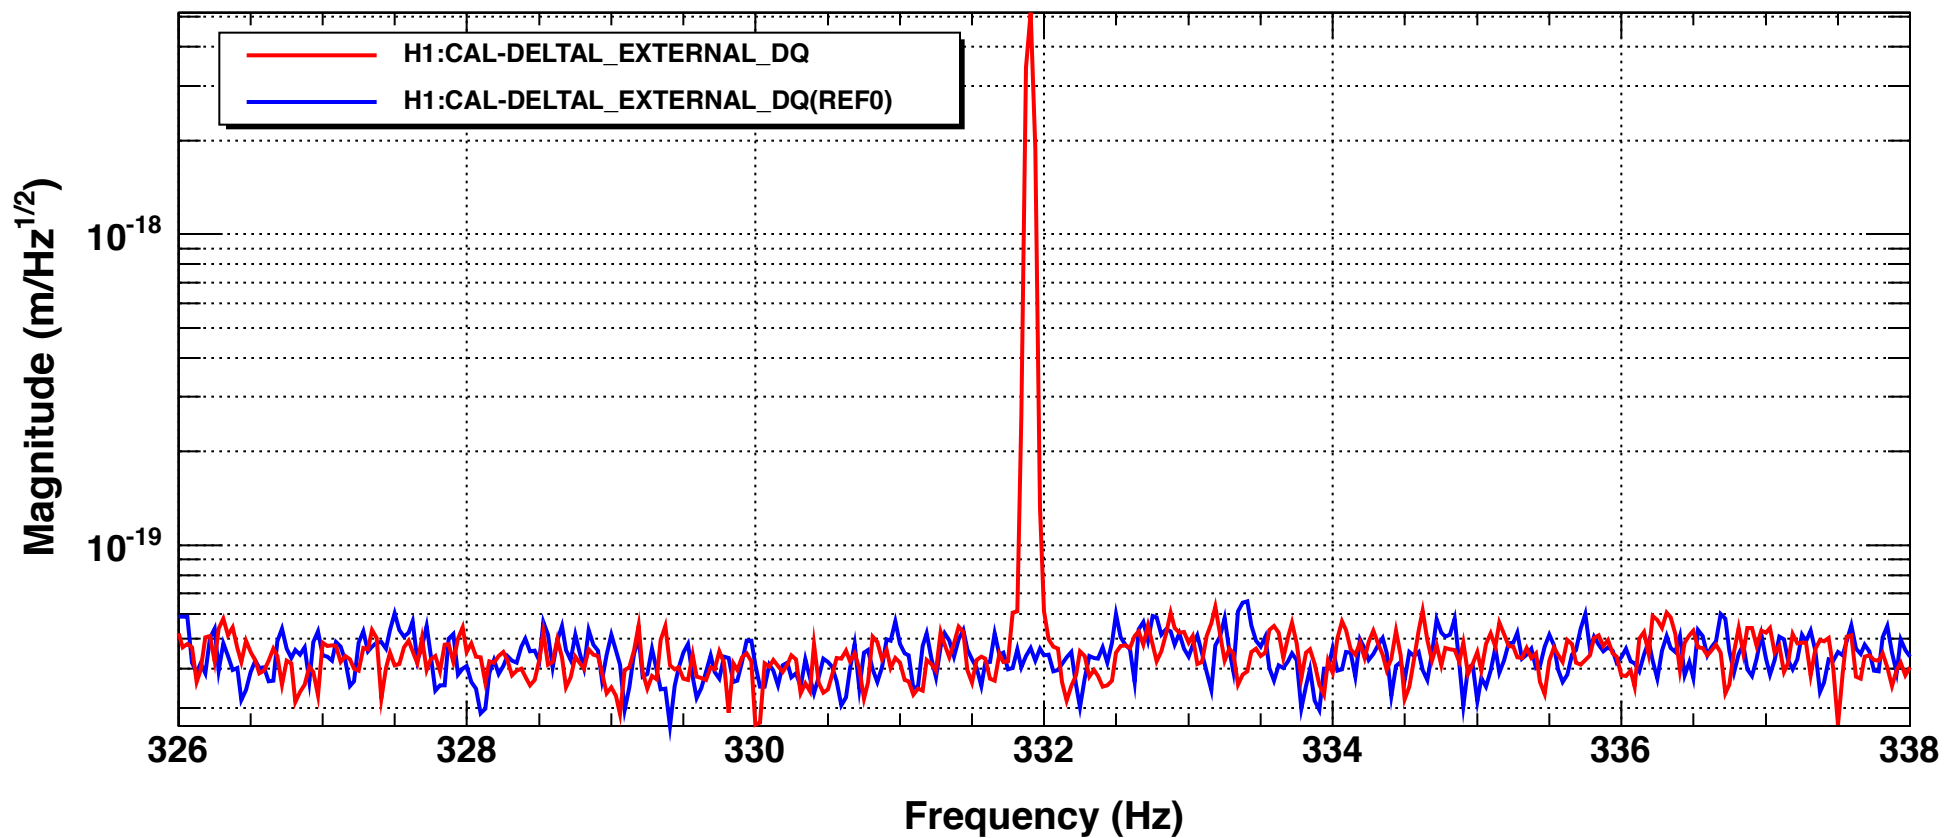

\*T0=11/09/2015 02:00:00

Avg=15

BW=0.0468742