


DARM: with and without Calibration lines

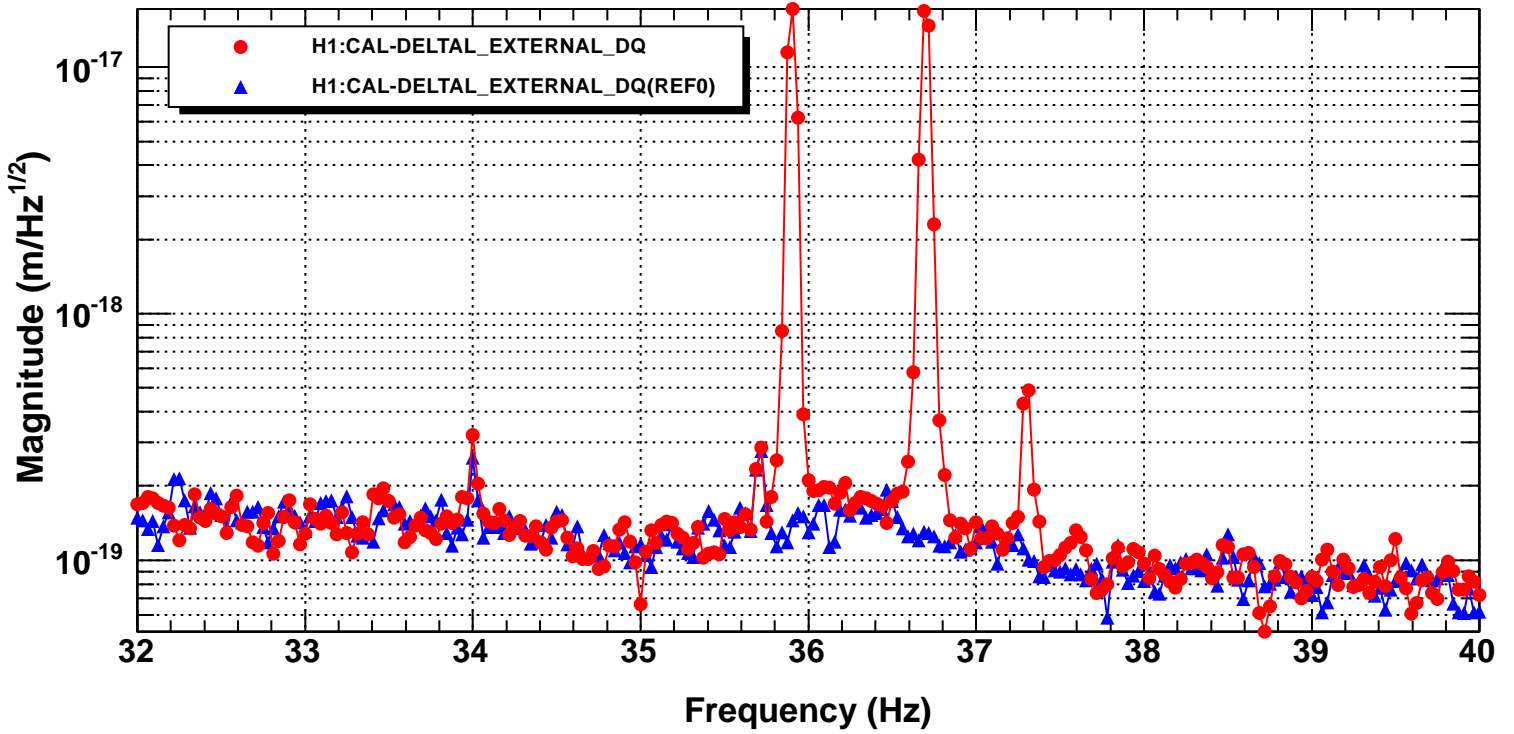


\*T0=11/09/2015 02:00:00

Avg=15

BW=0.0468742

DARM around first harmonic of calibration lines

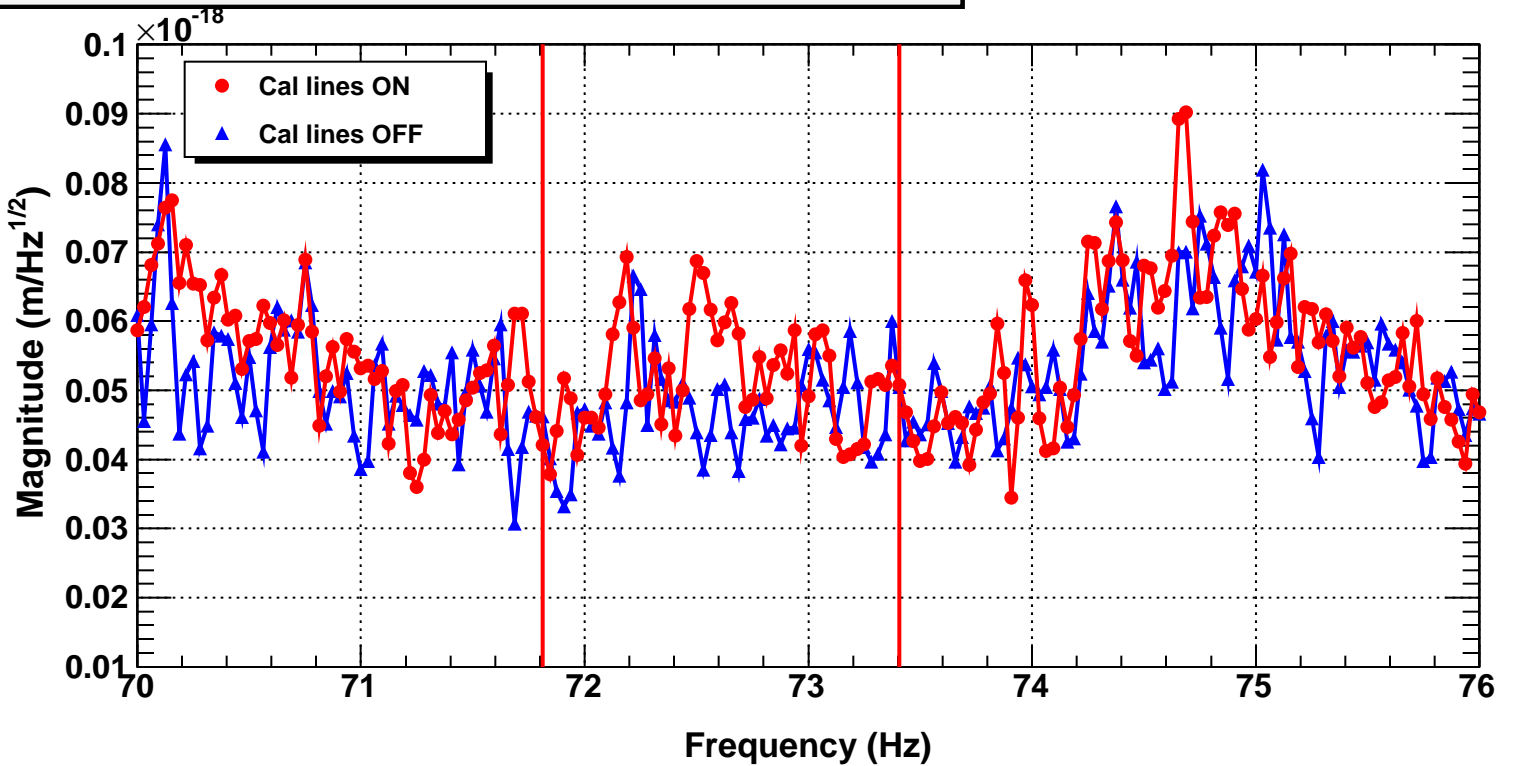

\*T0=11/09/2015 02:00:00

Avg=15

BW=0.0468742