
LHOX-End RxPD and TxPD Calibration Trends

Table of Contents

About	1
WS/TX Ratio when WS is at TX (Inner Beam)	2
WS/TX Ratio when WS is at TX (Outer Beam)	3
WS/TX Ratio when WS is at RX (Inner Beam)	4
WS/TX Ratio when WS is at RX (Outer Beam)	5
RX/TX Ratio (Inner Beam)	6
RX/TX Ratio (Outer Beam)	7
Optical Efficiency of Inner Beam	8
Optical Efficiency of Outer Beam	9
Total Optical Efficiency	10
TX/WS Ratio	11
RX/WS Ratio	12
TX/WS Ratio (Corrected for OE)	13
RX/WS Ratio (Corrected for OE)	14
Power Imbalance	15
Summary	16

About

This document contains the Pcal PD (TxPD and RxPD) Calibration trends. The first six section contains the six ratio measured at end-station labeled as m1, m2m6. The section that follows contains the relevant information calculated from these measurements which include Optical Efficiency, Power imbalance, TX/WS and RX/WS ratio.

Understanding Each Section

Each section contains a list of measurements with Magnitude, Standard Error and Relative Error for each measurement. The list is followed by two plot figure with Magnitude on the first plot and the the Normalized Magnitude on the second. Each Section ends with a Summary that contains the weighted mean of all the measurement along with their Standard deviation, Std Err and Rel Err where each of these terms are defined as:


$$\begin{aligned} \text{Mean} &= \text{sum}(x(i)*w(i))/\text{sum}(w(i)) \\ \text{Std Dev} &= \text{sqrt}(\text{sum}(w(i)*(x(i)-x_mean)^2)/((n-1)/n*\text{sum}(w(i)))) \\ \text{Std Err} &= \text{Std Dev}/\text{sqrt}(n) \\ \text{Rel Err} &= \text{Std Err}/\text{Mean} \end{aligned}$$

Report created on 22-Sep-2016

WS/TX Ratio when WS is at TX (Inner Beam)

List of Measurements

<i>Date</i>	<i>$m1 \pm SE_{\{m1\}}$</i>	<i>Normalized</i>
<i>D20150804</i>	<i>-0.158554 ± 0.000007</i>	<i>(1 ± 0.000042)</i>
<i>D20150827</i>	<i>-0.158839 ± 0.000004</i>	<i>(1 ± 0.000028)</i>
<i>D20151013</i>	<i>-0.158837 ± 0.000005</i>	<i>(1 ± 0.000032)</i>
<i>D20160108</i>	<i>-0.157751 ± 0.000005</i>	<i>(1 ± 0.000035)</i>
<i>D20160505</i>	<i>-0.158272 ± 0.000005</i>	<i>(1 ± 0.000034)</i>
<i>D20160628</i>	<i>-0.158053 ± 0.000005</i>	<i>(1 ± 0.000033)</i>
<i>D20160922</i>	<i>-0.157555 ± 0.000009</i>	<i>(1 ± 0.000060)</i>

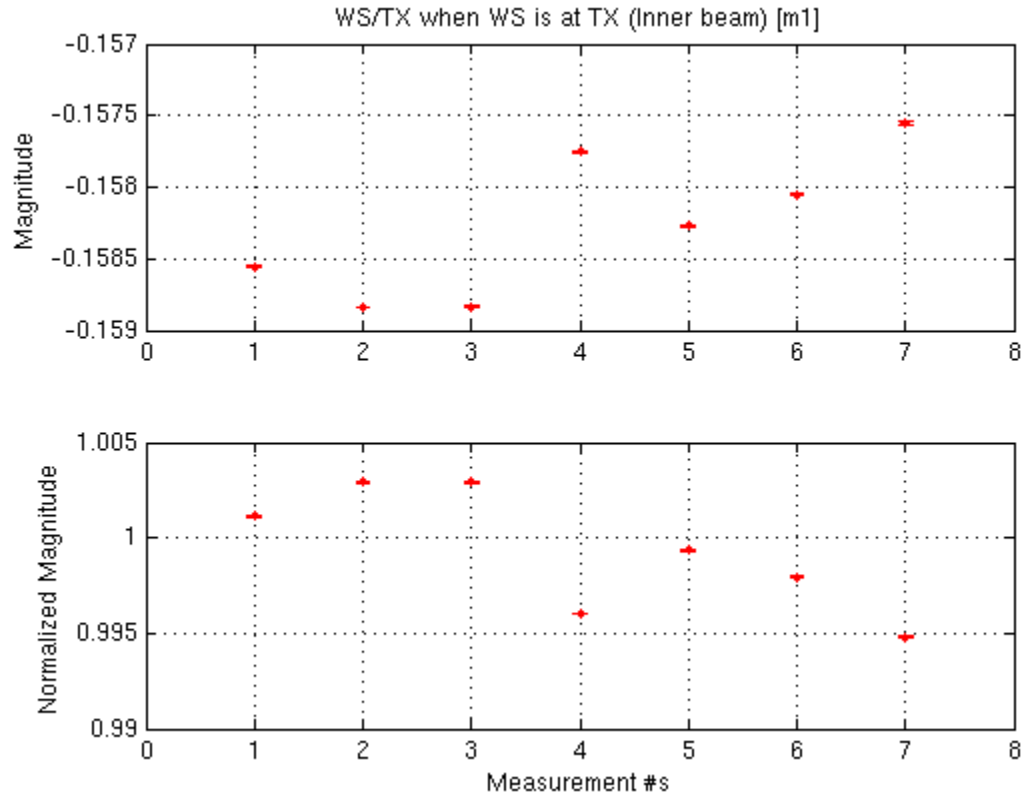


Summary of WS/TX when WS is at TX (Inner beam) [m1]:

Mean value: -0.158377
Standard deviation: 0.000480
Standard Error: 0.000195
Relative Standard Error: 0.001232

WS/TX Ratio when WS is at TX (Outer Beam)

List of Measurements

<i>Date</i>	<i>$m2 \pm SE_{\{m2\}}$</i>	<i>Normalized</i>
<i>D20150804</i>	<i>-0.158016 ± 0.000004</i>	<i>(1 ± 0.000027)</i>
<i>D20150827</i>	<i>-0.158288 ± 0.000004</i>	<i>(1 ± 0.000028)</i>
<i>D20151013</i>	<i>-0.158597 ± 0.000005</i>	<i>(1 ± 0.000030)</i>
<i>D20160108</i>	<i>-0.159262 ± 0.000005</i>	<i>(1 ± 0.000029)</i>
<i>D20160505</i>	<i>-0.158328 ± 0.000005</i>	<i>(1 ± 0.000033)</i>
<i>D20160628</i>	<i>-0.157681 ± 0.000005</i>	<i>(1 ± 0.000032)</i>
<i>D20160922</i>	<i>-0.158094 ± 0.000010</i>	<i>(1 ± 0.000062)</i>

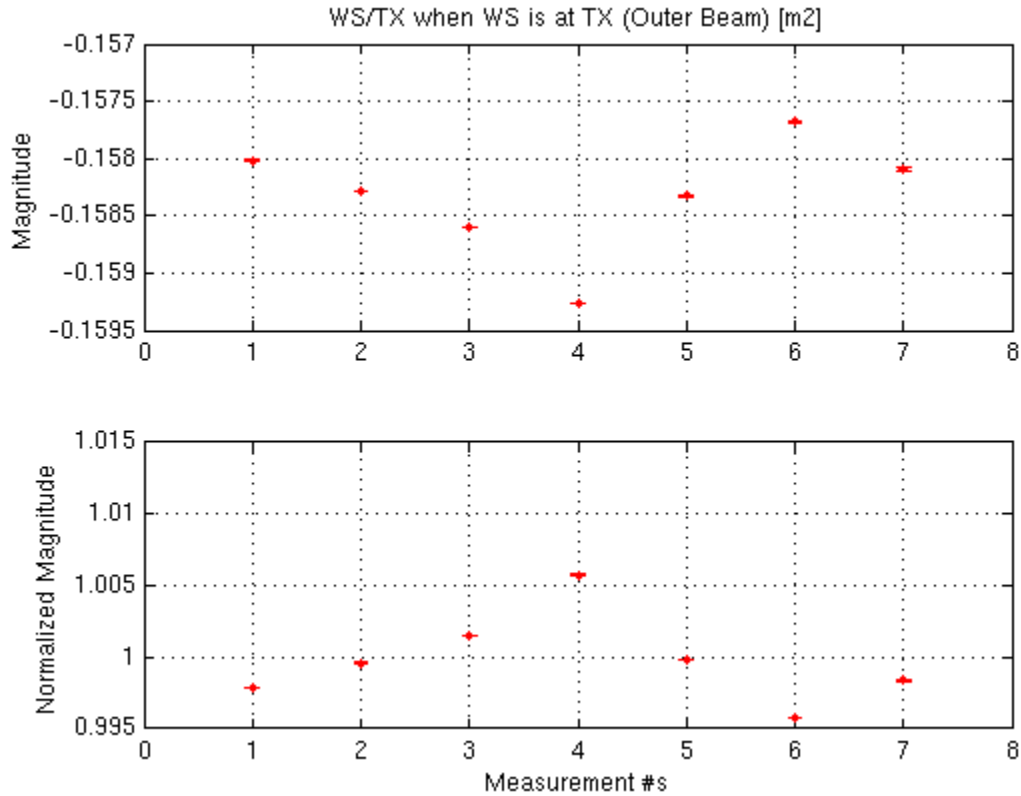


Summary of WS/TX when WS is at TX (Outer Beam) [m2]:
Mean value: -0.158353
Standard deviation: 0.000522

Standard Error: 0.000212
Relative Standard Error: 0.001341

WS/TX Ratio when WS is at RX (Inner Beam)

List of Measurements

Date	$m3 \pm SE_{\{m3\}}$	Normalized
D20150804	-0.156120 ± 0.000006	(1 ± 0.000039)
D20150827	-0.156101 ± 0.000005	(1 ± 0.000032)
D20151013	-0.154453 ± 0.000005	(1 ± 0.000034)
D20160108	-0.141148 ± 0.000008	(1 ± 0.000057)
D20160505	-0.132887 ± 0.000011	(1 ± 0.000081)
D20160628	-0.123153 ± 0.000009	(1 ± 0.000073)
D20160922	-0.155734 ± 0.000009	(1 ± 0.000060)

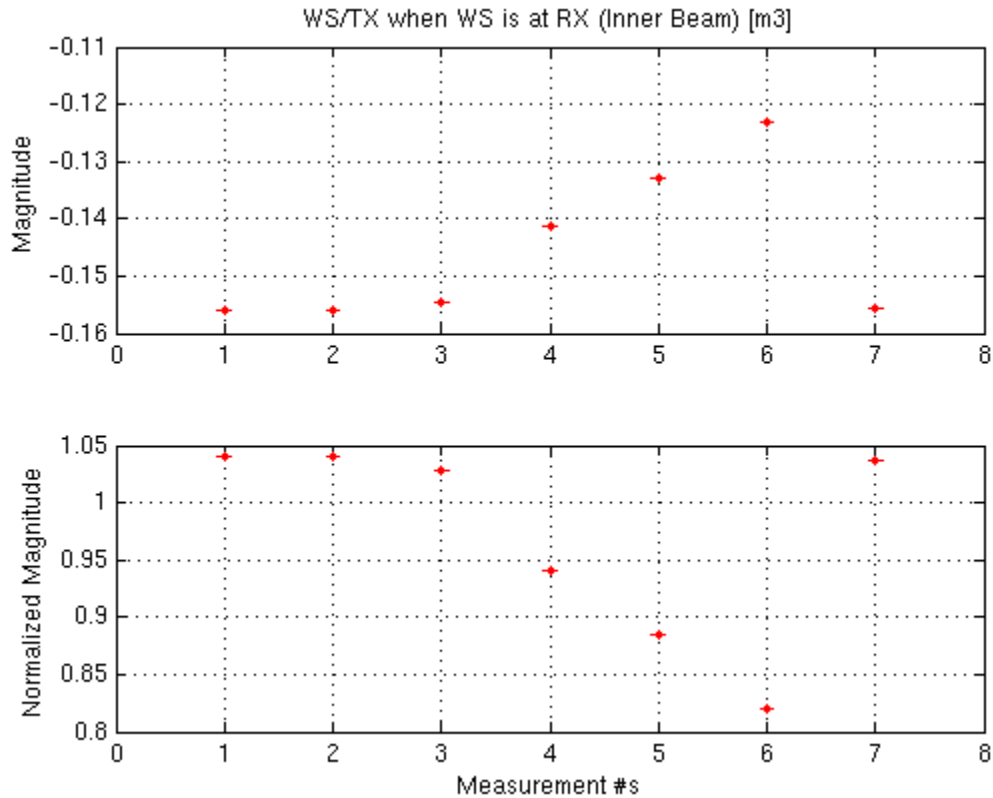


Summary of WS/TX when WS is at RX (Inner Beam) [m3]:

Mean value: -0.150112
Standard deviation: 0.011205
Standard Error: 0.004560
Relative Standard Error: 0.030378

WS/TX Ratio when WS is at RX (Outer Beam)

List of Measurements

Date	$m4 \pm SE_{\{m4\}}$	Normalized
D20150804	-0.154938 ± 0.000006	(1 ± 0.000038)
D20150827	-0.153203 ± 0.000005	(1 ± 0.000031)
D20151013	-0.140688 ± 0.000010	(1 ± 0.000068)
D20160108	-0.107301 ± 0.000014	(1 ± 0.000127)
D20160505	-0.096847 ± 0.000018	(1 ± 0.000181)
D20160628	-0.072041 ± 0.000018	(1 ± 0.000253)
D20160922	-0.156012 ± 0.000009	(1 ± 0.000061)

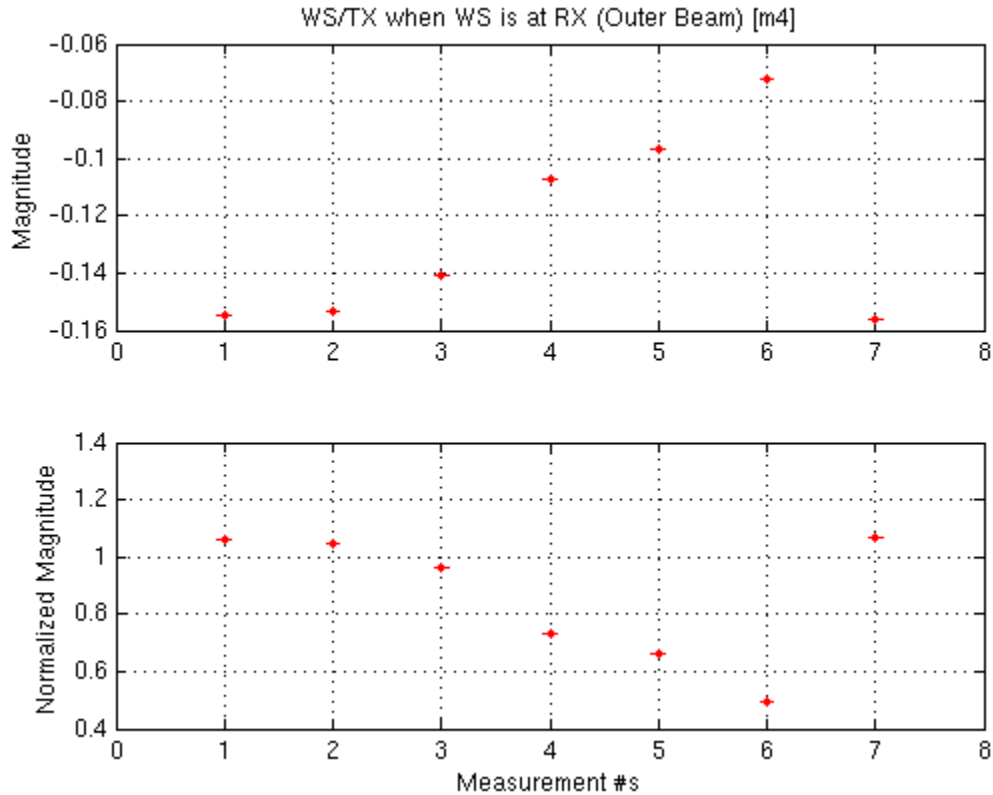


Summary of WS/TX when WS is at RX (Outer Beam) [m4]:

Mean value: -0.146483
Standard deviation: 0.020338
Standard Error: 0.008277
Relative Standard Error: 0.056502

RX/TX Ratio (Inner Beam)

List of Measurements

<i>Date</i>	<i>m5 ± SE_{m5}</i>	<i>Normalized</i>
<i>D20150804</i>	<i>0.628735 ± 0.000004</i>	<i>(1 ± 0.000006)</i>
<i>D20150827</i>	<i>0.627025 ± 0.000003</i>	<i>(1 ± 0.000005)</i>
<i>D20151013</i>	<i>0.620693 ± 0.000007</i>	<i>(1 ± 0.000011)</i>
<i>D20160108</i>	<i>0.570708 ± 0.000023</i>	<i>(1 ± 0.000040)</i>
<i>D20160505</i>	<i>0.533749 ± 0.000043</i>	<i>(1 ± 0.000080)</i>
<i>D20160628</i>	<i>0.487934 ± 0.000054</i>	<i>(1 ± 0.000112)</i>
<i>D20160922</i>	<i>0.627214 ± 0.000006</i>	<i>(1 ± 0.000010)</i>

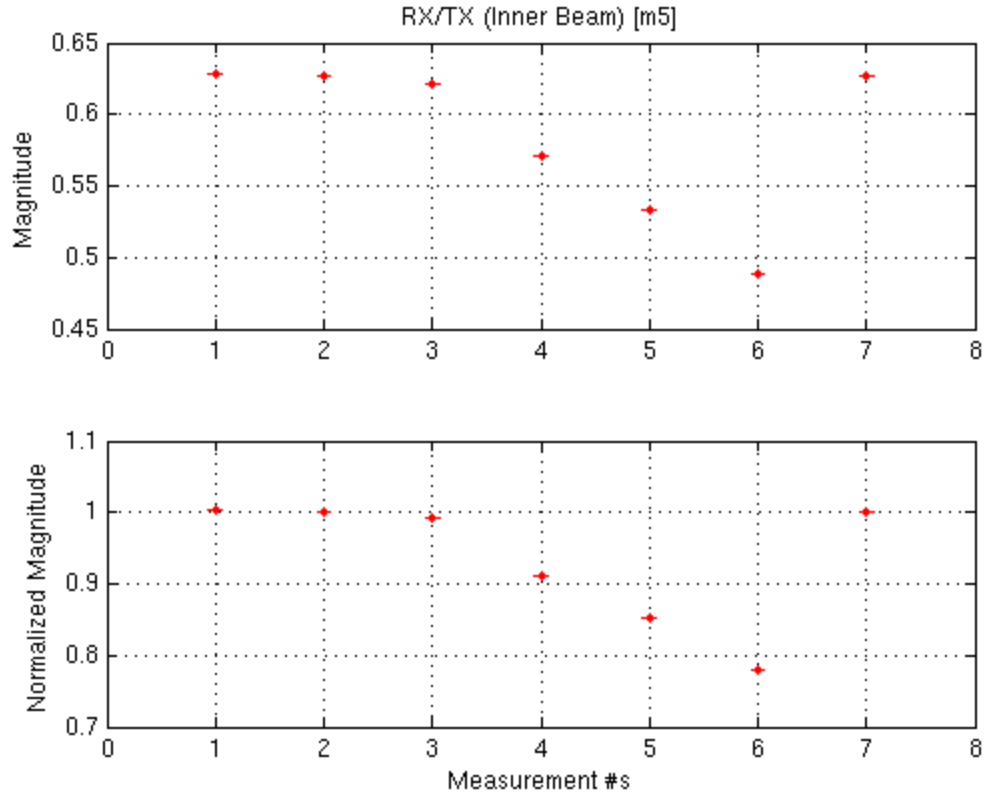


Summary of RX/TX (Inner Beam) [m5]:

Mean value: 0.626090
 Standard deviation: 0.009699
 Standard Error: 0.003947
 Relative Standard Error: 0.006305

RX/TX Ratio (Outer Beam)

List of Measurements

Date	$m6 \pm SE_{\{m6\}}$	Normalized
D20150804	0.623505 ± 0.000005	(1 ± 0.000008)
D20150827	0.612750 ± 0.000015	(1 ± 0.000024)
D20151013	0.563327 ± 0.000033	(1 ± 0.000059)
D20160108	0.429049 ± 0.000052	(1 ± 0.000122)
D20160505	0.382774 ± 0.000063	(1 ± 0.000164)
D20160628	0.278553 ± 0.000088	(1 ± 0.000315)
D20160922	0.628100 ± 0.000003	(1 ± 0.000005)

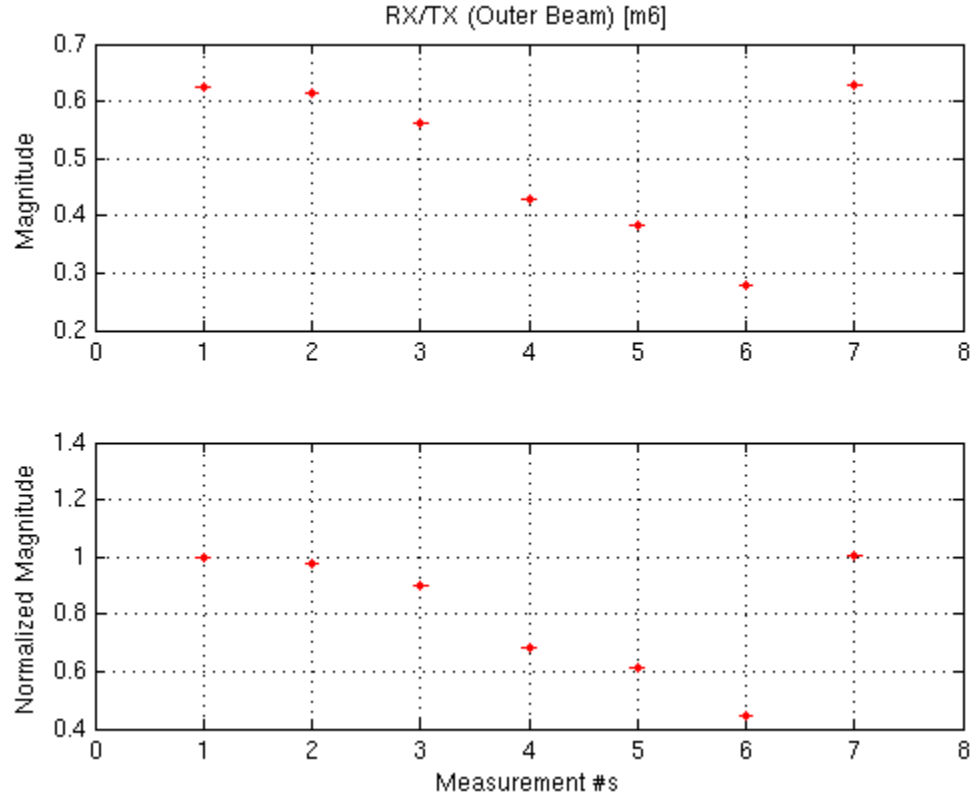

Summary of RX/TX (Outer Beam) [m6]:

Mean value: 0.625125
Standard deviation: 0.019067
Standard Error: 0.007760
Relative Standard Error: 0.012413

Optical Efficiency of Inner Beam


List of Measurements

Date	$e_i \pm SE_{\{e_i\}}$	Normalized
D20150804	0.984647 ± 0.000058	(1 ± 0.000058)
D20150827	0.982762 ± 0.000043	(1 ± 0.000043)
D20151013	0.972403 ± 0.000046	(1 ± 0.000048)
D20160108	0.894753 ± 0.000066	(1 ± 0.000074)
D20160505	0.839608 ± 0.000088	(1 ± 0.000105)
D20160628	0.779192 ± 0.000080	(1 ± 0.000103)

D20160922

0.988443 ± 0.000085

(1 ± 0.000086)

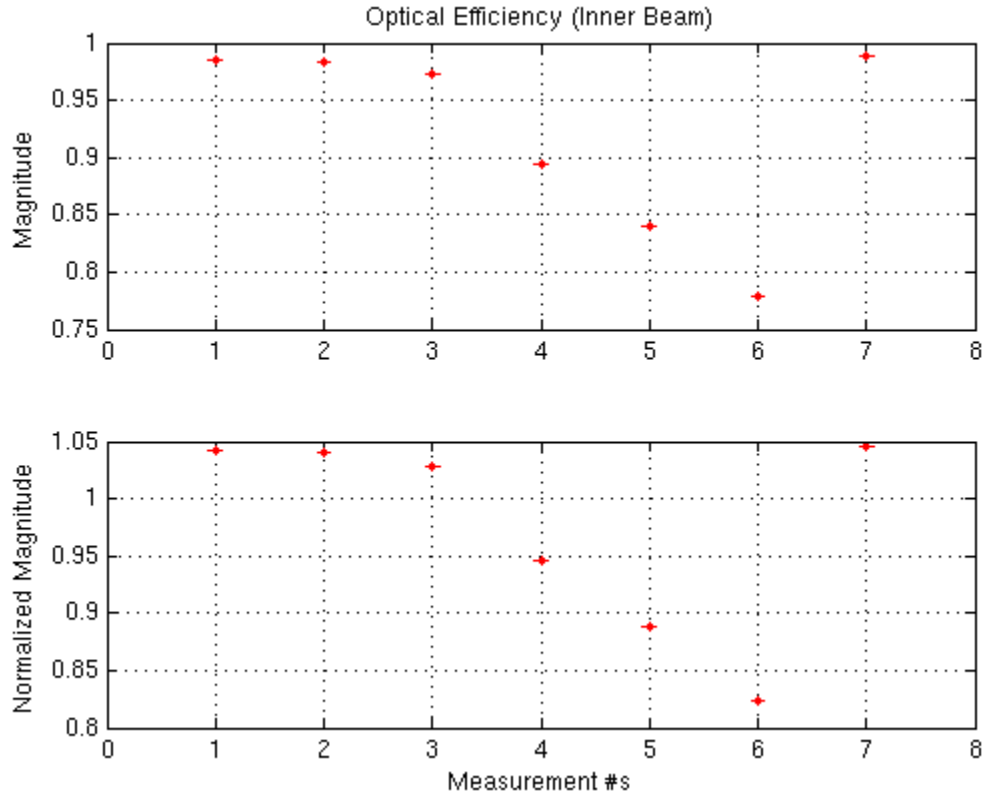

Summary of Optical Efficiency (Inner Beam):


Mean value: 0.945343
Standard deviation: 0.069582
Standard Error: 0.028317
Relative Standard Error: 0.029954

Optical Efficiency of Outer Beam

List of Measurements

Date	$e_o \pm SE_{\{e_o\}}$	Normalized
D20150804	0.980522 ± 0.000046	(1 ± 0.000047)
D20150827	0.967879 ± 0.000042	(1 ± 0.000043)
D20151013	0.887079 ± 0.000074	(1 ± 0.000083)
D20160108	0.673740 ± 0.000130	(1 ± 0.000193)
D20160505	0.611689 ± 0.000184	(1 ± 0.000301)

<i>D20160628</i>	<i>0.456880 ± 0.000255</i>	<i>(1 ± 0.000557)</i>
<i>D20160922</i>	<i>0.986835 ± 0.000087</i>	<i>(1 ± 0.000088)</i>

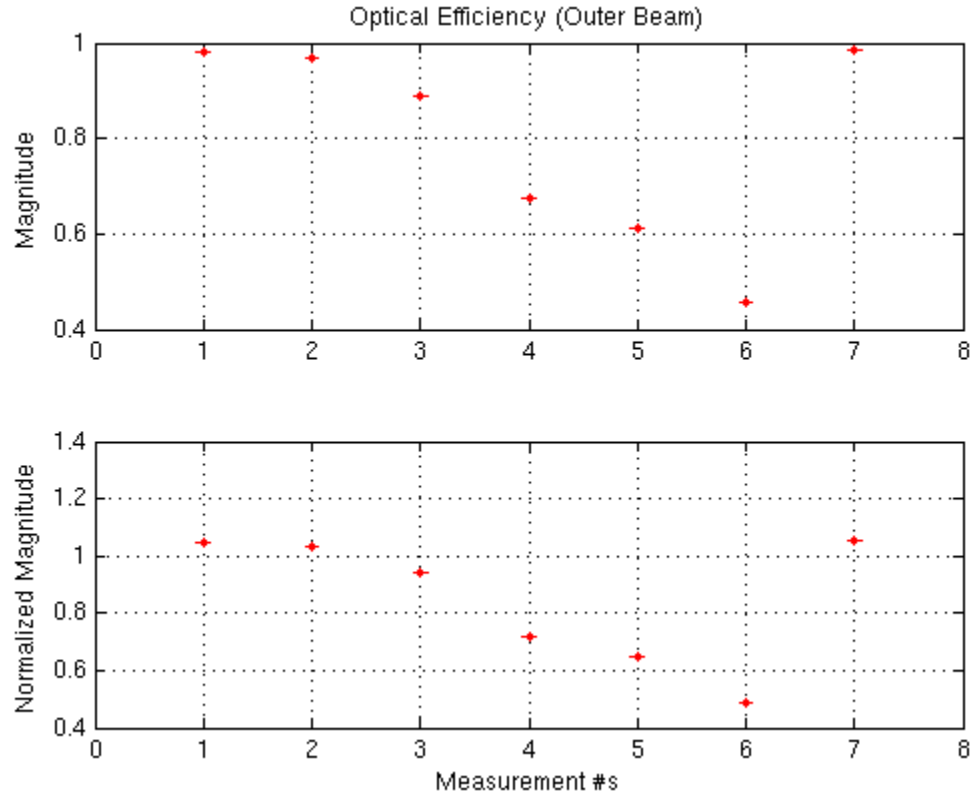

Summary of Optical Efficiency (Outer Beam):


<i>Mean value:</i>	<i>0.938987</i>
<i>Standard deviation:</i>	<i>0.101905</i>
<i>Standard Error:</i>	<i>0.041471</i>
<i>Relative Standard Error:</i>	<i>0.044166</i>

Total Optical Efficiency

List of Measurements

<i>Date</i>	<i>e ± SE_{e}</i>	<i>Normalized</i>
<i>D20150804</i>	<i>0.982588 ± 0.000036</i>	<i>(1 ± 0.000037)</i>
<i>D20150827</i>	<i>0.975333 ± 0.000029</i>	<i>(1 ± 0.000030)</i>
<i>D20151013</i>	<i>0.929774 ± 0.000040</i>	<i>(1 ± 0.000043)</i>
<i>D20160108</i>	<i>0.783720 ± 0.000053</i>	<i>(1 ± 0.000067)</i>

<i>D20160505</i>	<i>0.725628 ± 0.000067</i>	<i>(1 ± 0.000093)</i>
<i>D20160628</i>	<i>0.618226 ± 0.000066</i>	<i>(1 ± 0.000106)</i>
<i>D20160922</i>	<i>0.987638 ± 0.000060</i>	<i>(1 ± 0.000061)</i>

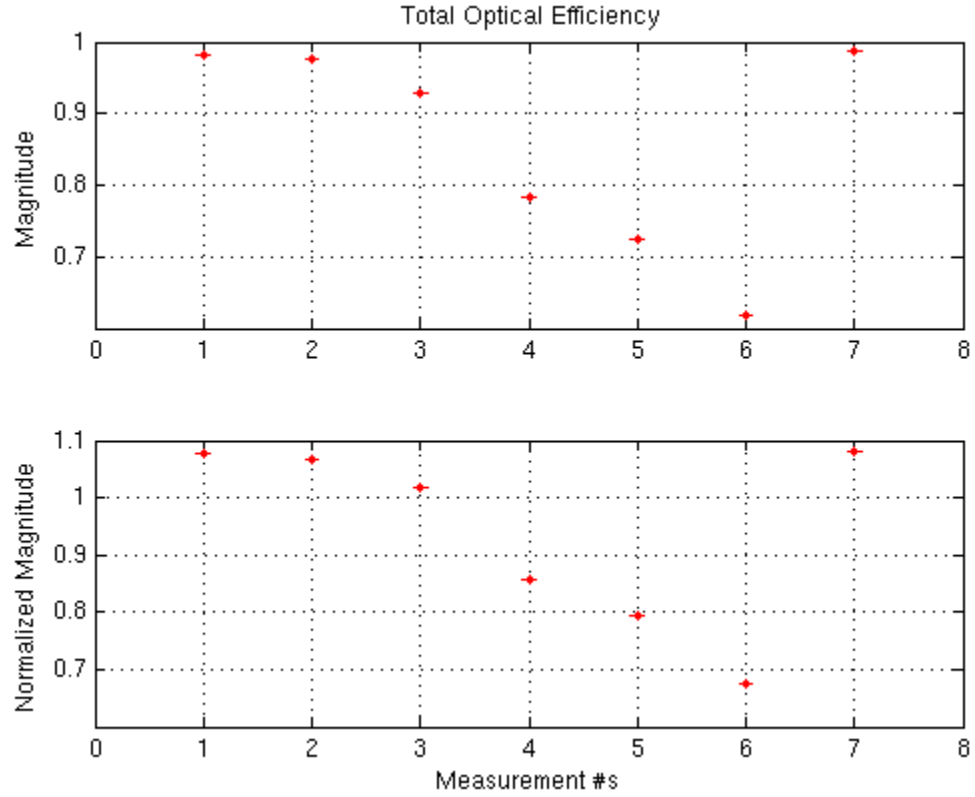

Summary of Total Optical Efficiency:


<i>Mean value:</i>	<i>0.913555</i>
<i>Standard deviation:</i>	<i>0.118153</i>
<i>Standard Error:</i>	<i>0.048083</i>
<i>Relative Standard Error:</i>	<i>0.052633</i>

TX/WS Ratio

List of Measurements

<i>Date</i>	<i>R_TW ± SE_{R_TW}</i>	<i>Normalized</i>
<i>D20150804</i>	<i>-3.158856 ± 0.000008</i>	<i>(1 ± 0.000003)</i>
<i>D20150827</i>	<i>-3.153314 ± 0.000006</i>	<i>(1 ± 0.000002)</i>
<i>D20151013</i>	<i>-3.150260 ± 0.000007</i>	<i>(1 ± 0.000002)</i>

<i>D20160108</i>	<i>-3.154444 ± 0.000007</i>	<i>(1 ± 0.000002)</i>
<i>D20160505</i>	<i>-3.158561 ± 0.000008</i>	<i>(1 ± 0.000002)</i>
<i>D20160628</i>	<i>-3.167227 ± 0.000007</i>	<i>(1 ± 0.000002)</i>
<i>D20160922</i>	<i>-3.168082 ± 0.000014</i>	<i>(1 ± 0.000004)</i>

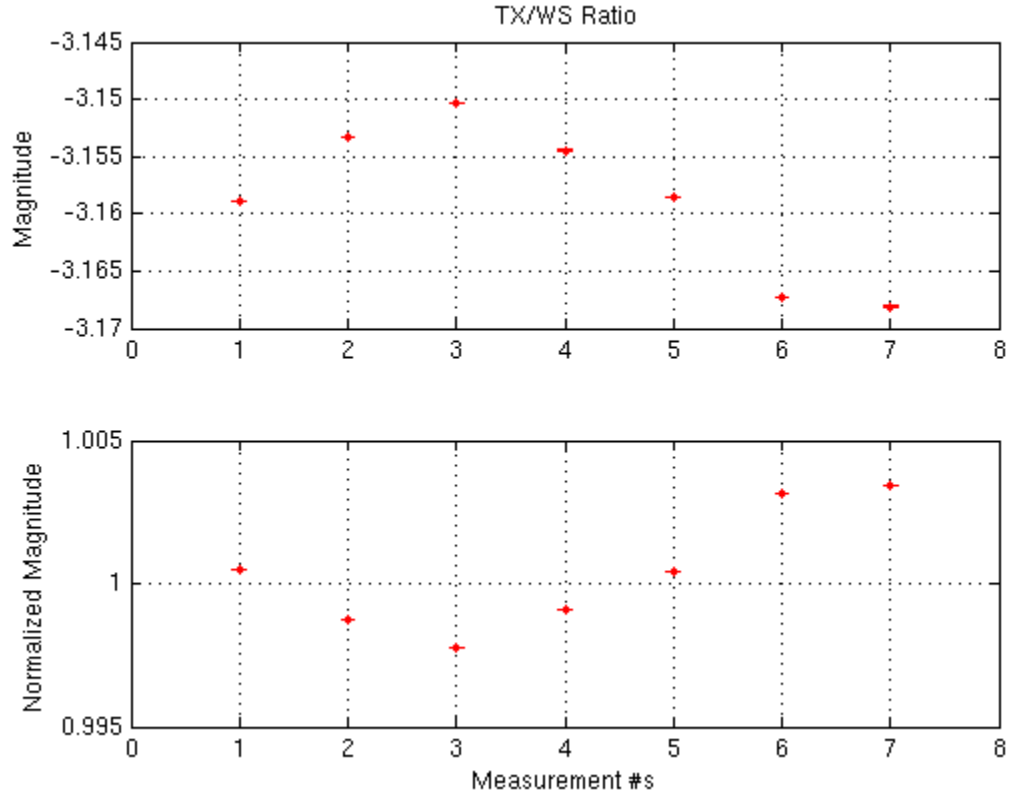

Summary of TX/WS Ratio:


Mean value:	-3.157232
Standard deviation:	0.006302
Standard Error:	0.002565
Relative Standard Error:	0.000812

RX/WS Ratio

List of Measurements

<i>Date</i>	<i>R_{RW} ± SE_{R_{RW}}</i>	<i>Normalized</i>
<i>D20150804</i>	<i>-4.025735 ± 0.000111</i>	<i>(1 ± 0.000028)</i>
<i>D20150827</i>	<i>-4.008193 ± 0.000102</i>	<i>(1 ± 0.000025)</i>

<i>D20151013</i>	<i>-4.011358 ± 0.000194</i>	<i>(1 ± 0.000048)</i>
<i>D20160108</i>	<i>-4.020935 ± 0.000378</i>	<i>(1 ± 0.000094)</i>
<i>D20160505</i>	<i>-3.984463 ± 0.000534</i>	<i>(1 ± 0.000134)</i>
<i>D20160628</i>	<i>-3.914288 ± 0.000823</i>	<i>(1 ± 0.000210)</i>
<i>D20160922</i>	<i>-4.026718 ± 0.000174</i>	<i>(1 ± 0.000043)</i>

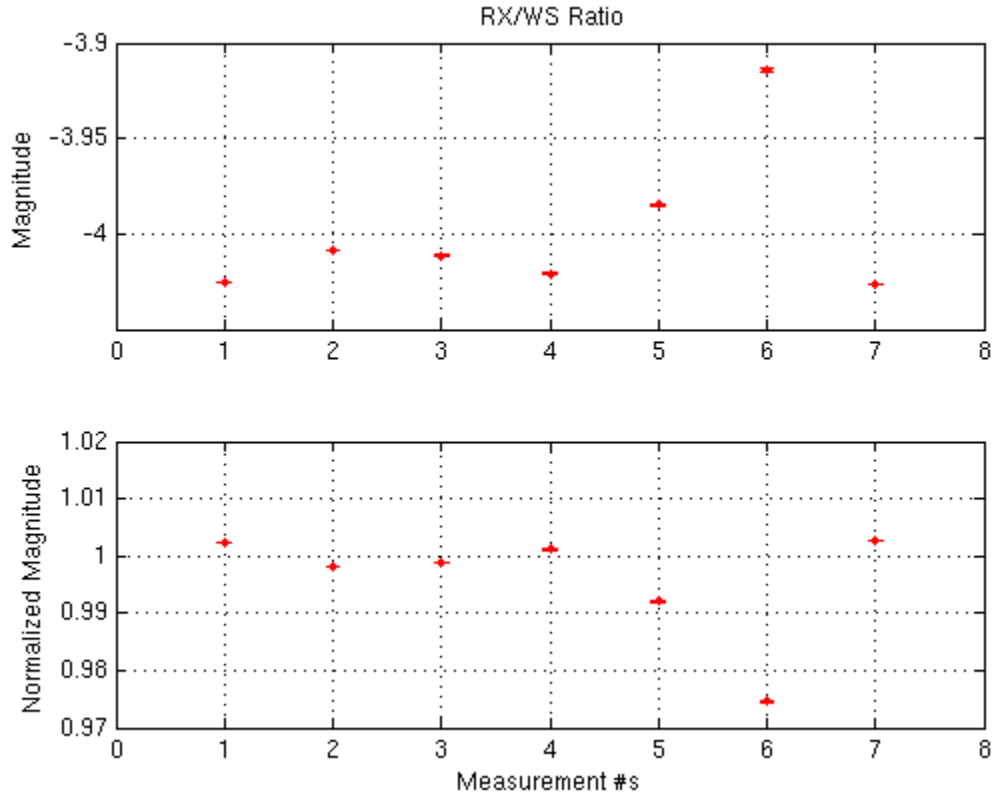

Summary of RX/WS Ratio:


<i>Mean value:</i>	<i>-4.016161</i>
<i>Standard deviation:</i>	<i>0.013125</i>
<i>Standard Error:</i>	<i>0.005342</i>
<i>Relative Standard Error:</i>	<i>0.001330</i>

TX/WS Ratio (Corrected for OE)

List of Measurements

<i>Date</i>	<i>R_Twc ± SE_{R_Twc}</i>	<i>Normalized</i>
<i>D20150804</i>	<i>-3.186598 ± 0.000059</i>	<i>(1 ± 0.000018)</i>

D20150827	-3.192691 ± 0.000047	(1 ± 0.000015)
D20151013	-3.264901 ± 0.000069	(1 ± 0.000021)
D20160108	-3.536928 ± 0.000108	(1 ± 0.000031)
D20160505	-3.660766 ± 0.000147	(1 ± 0.000040)
D20160628	-3.914444 ± 0.000165	(1 ± 0.000042)
D20160922	-3.187786 ± 0.000097	(1 ± 0.000030)

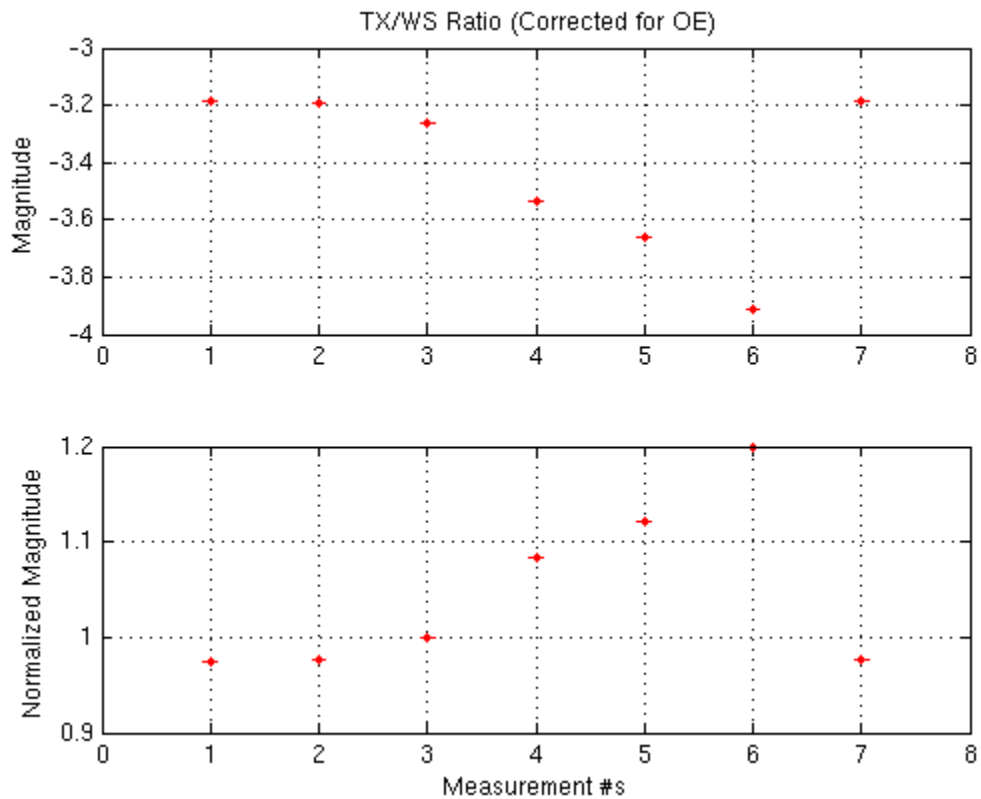

Summary of TX/WS Ratio (Corrected for OE):


Mean value:	-3.266975
Standard deviation:	0.179790
Standard Error:	0.073167
Relative Standard Error:	0.022396

RX/WS Ratio (Corrected for OE)

List of Measurements

Date	$R_{Rwc} \pm SE_{\{R_{Rwc}\}}$	Normalized
------	--------------------------------	------------

D20150804	-3.990379 ± 0.000076	(1 ± 0.000019)
D20150827	-3.958141 ± 0.000077	(1 ± 0.000019)
D20151013	-3.865381 ± 0.000143	(1 ± 0.000037)
D20160108	-3.533387 ± 0.000260	(1 ± 0.000073)
D20160505	-3.350941 ± 0.000347	(1 ± 0.000104)
D20160628	-2.990824 ± 0.000536	(1 ± 0.000179)
D20160922	-4.001674 ± 0.000123	(1 ± 0.000031)

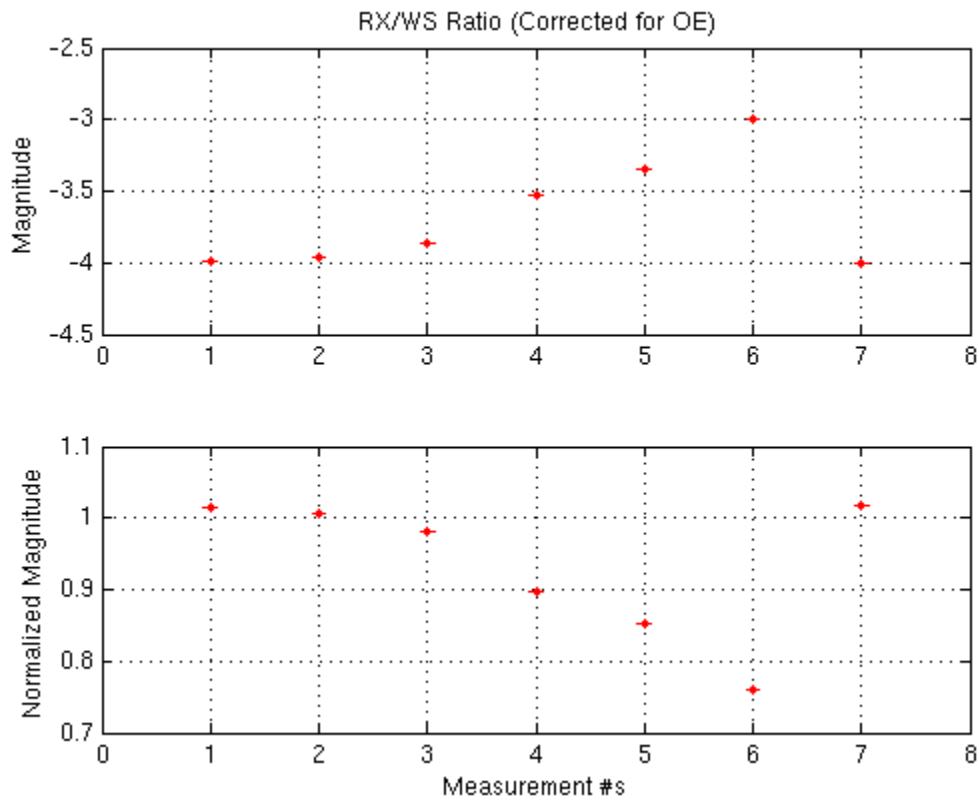

Summary of RX/WS Ratio (Corrected for OE):


Mean value:	-3.935577
Standard deviation:	0.151549
Standard Error:	0.061674
Relative Standard Error:	0.015671

Power Imbalance

List of Measurements

LHOX-End RxPD and Tx-
PD Calibration Trends

D20150804	1.003523 ± 0.000051	(1 ± 0.000051)
D20150827	1.003430 ± 0.000040	(1 ± 0.000040)
D20151013	1.001645 ± 0.000043	(1 ± 0.000043)
D20160108	0.990394 ± 0.000045	(1 ± 0.000045)
D20160505	0.999665 ± 0.000048	(1 ± 0.000048)
D20160628	1.002389 ± 0.000046	(1 ± 0.000046)
D20160922	0.996618 ± 0.000047	(1 ± 0.000047)

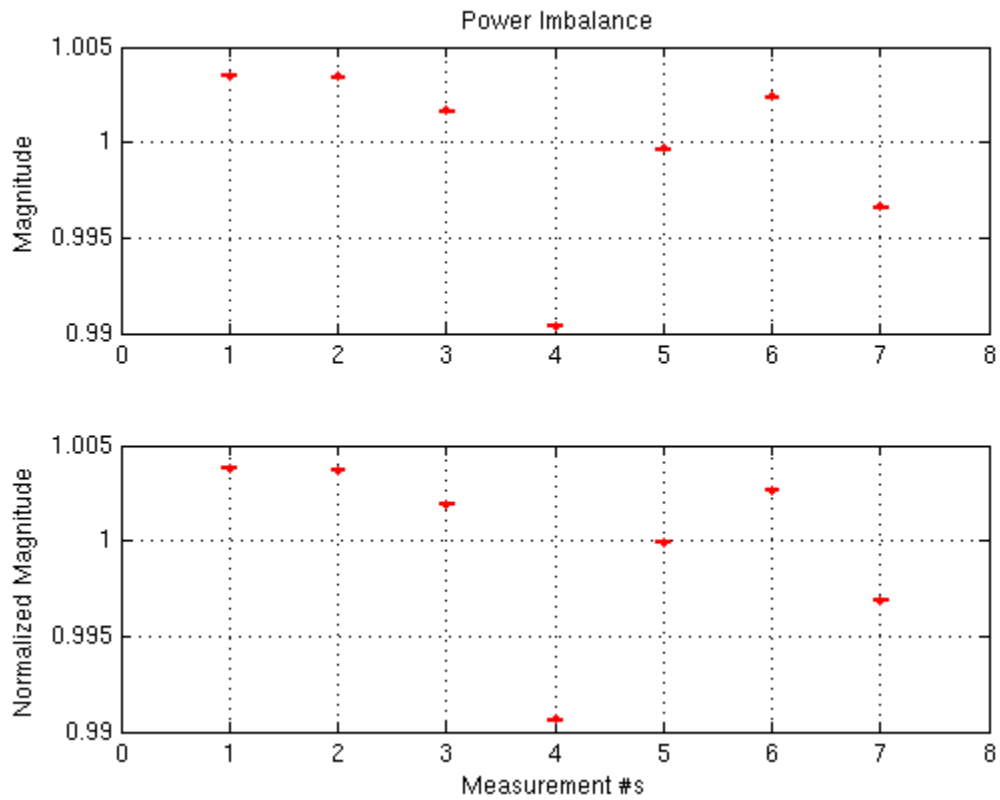

Summary of Power Imbalance:

Mean value:	0.999722
Standard deviation:	0.004793
Standard Error:	0.001951
Relative Standard Error:	0.001951

Summary

Description	Value	Std Dev	Std Err	Rel Err:
OE (e)	0.9136	0.1182	0.0481	0.0526

LHOX-End RxPD and Tx-
PD Calibration Trends

<i>TX/WS (a1a2)</i>	<i>-3.2670</i>	<i>0.1798</i>	<i>0.0732</i>	<i>0.0224</i>
<i>RX/WS (b1b2)</i>	<i>-3.9356</i>	<i>0.1515</i>	<i>0.0617</i>	<i>0.0157</i>
<i>W (a5)</i>	<i>1.0000</i>	<i>----</i>	<i>----</i>	<i>0.0250</i>

Published with MATLAB® 8.0