


11-1-2016 11:40 am

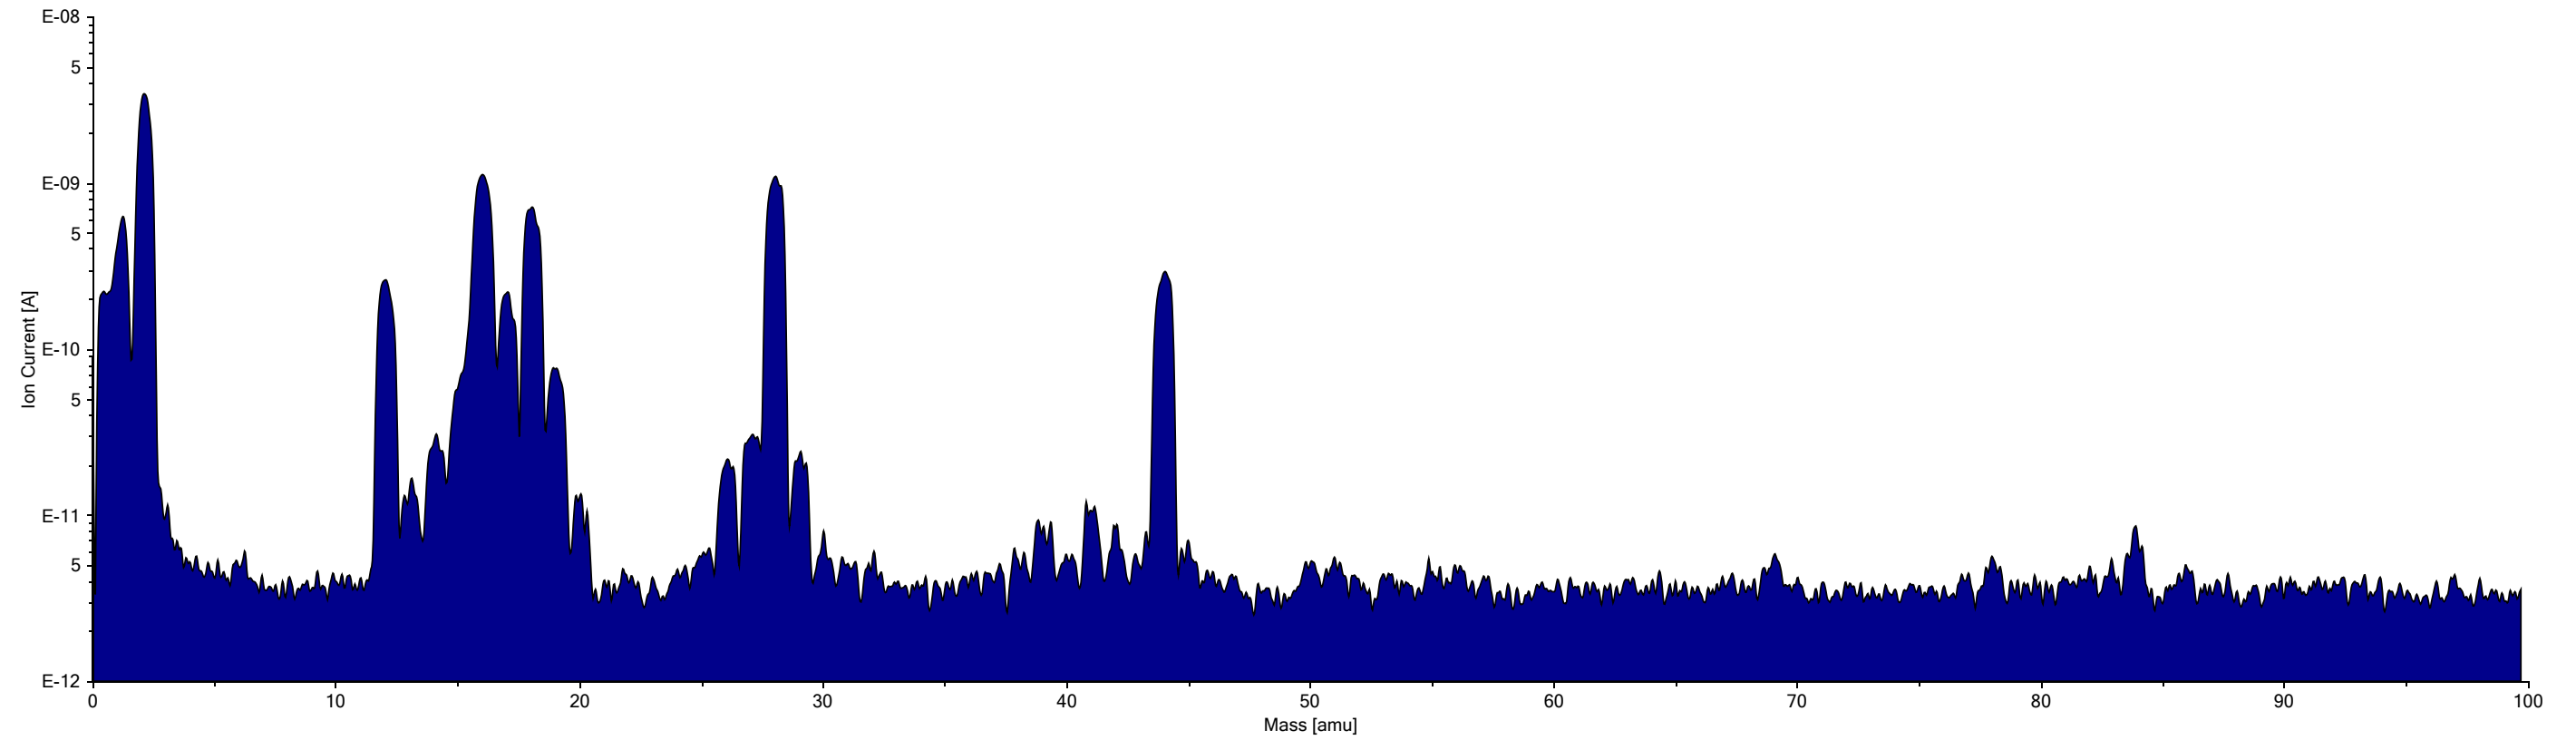

X-end RGA, isolated from X-end volume, pumped by locally mounted turbo (~10 l/s net), calibration gases isolated, SEM = 1500 volts and with factory default ionizer settings