


11-1-2016 12:00 pm

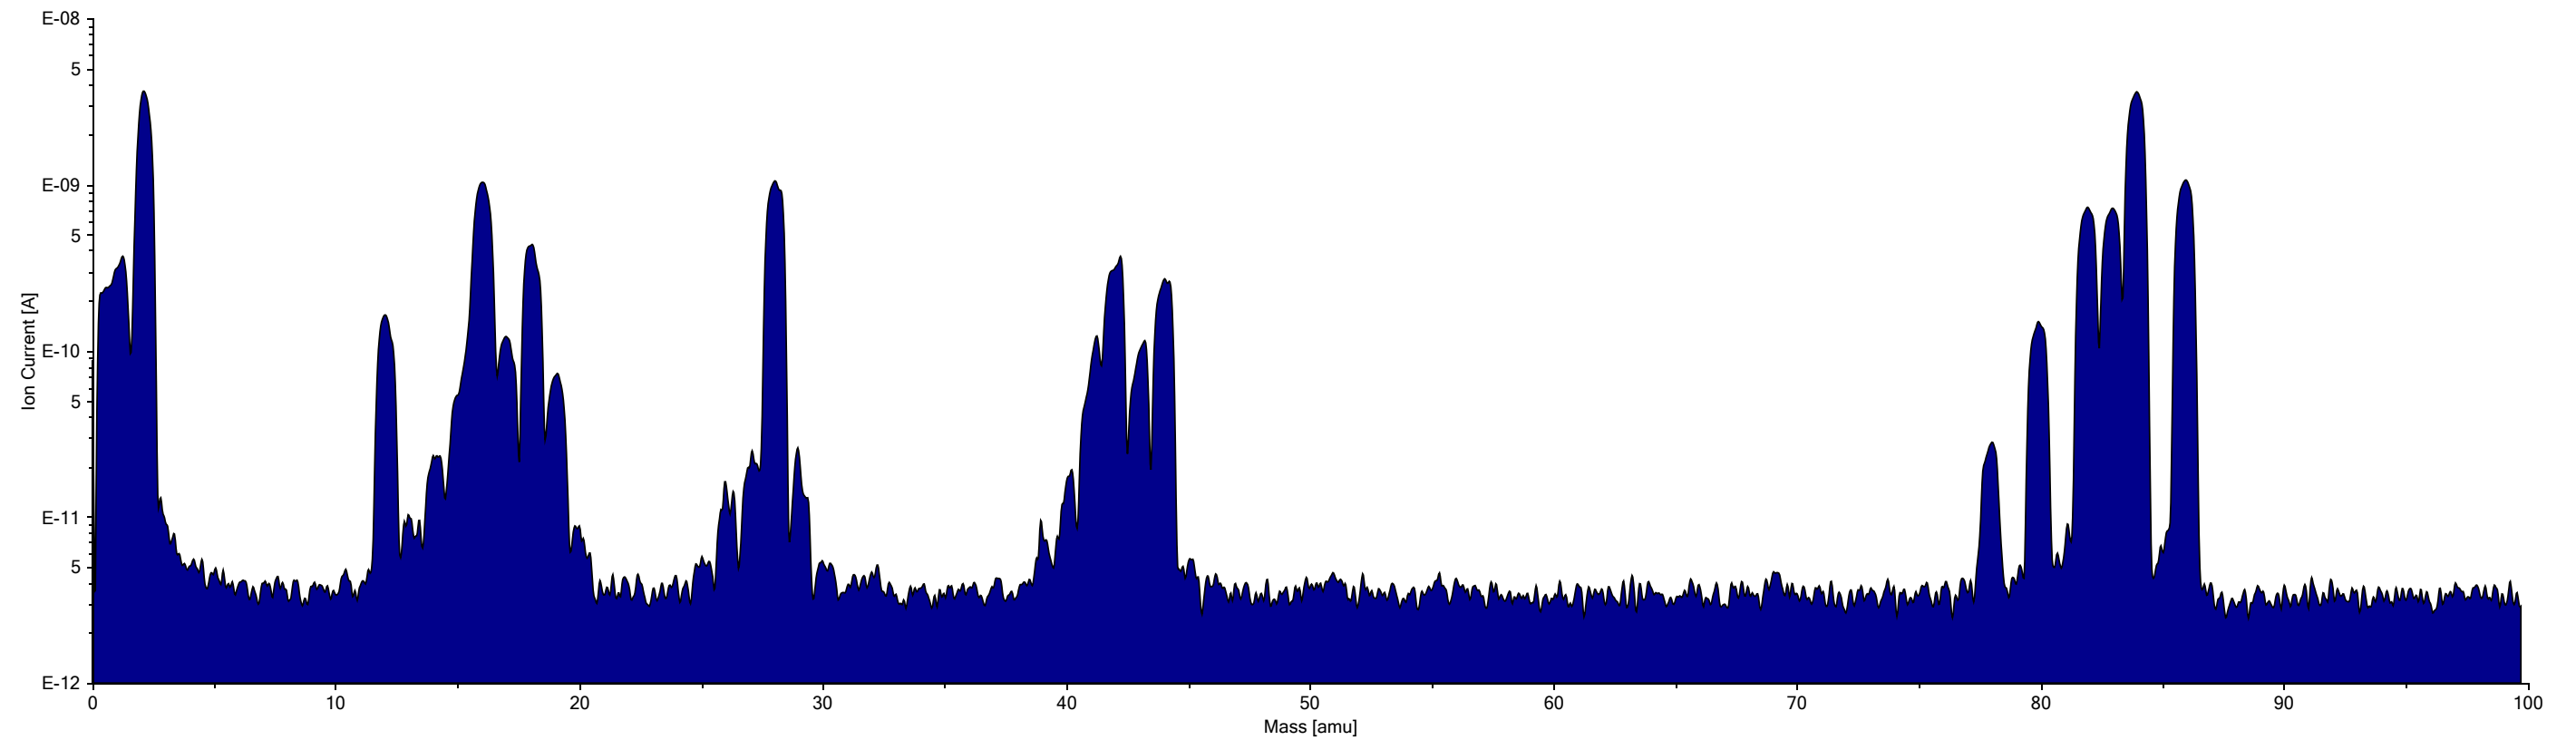

X-end RGA, isolated from X-end volume, pumped by locally mounted turbo (~10 l/s net),  
Kr calibration gas open ( $5 \times 10^{-8}$  torr\*l/sec), SEM = 1500 volts and with factory default  
ionizer settings