


11-1-2016 12:13 pm

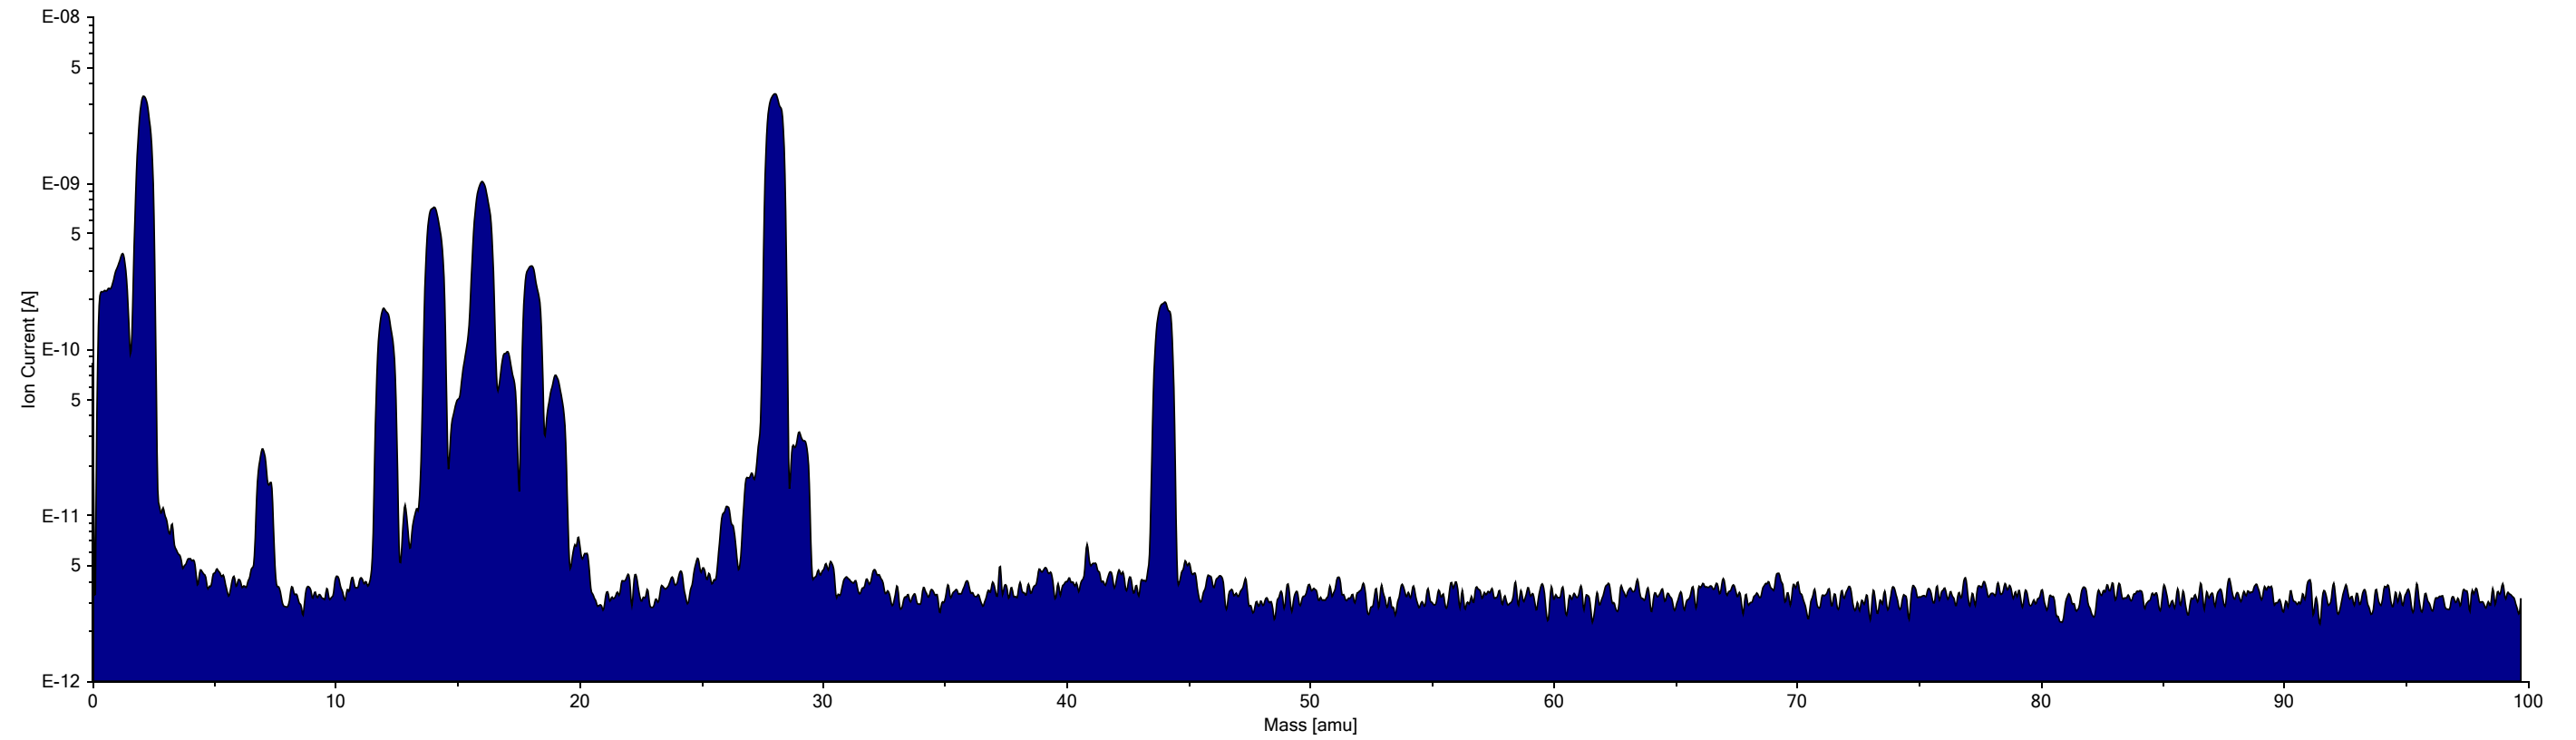

X-end RGA, isolated from X-end volume, pumped by locally mounted turbo (10 l/s net), N2 calibration gas open (5×10^{-8} torr*l/sec), SEM = 1500 volts and with factory default ionizer settings