
LHOY-End RxPD and TxPD Calibration Trends

Table of Contents

About	1
WS/TX Ratio when WS is at TX (Inner Beam)	2
WS/TX Ratio when WS is at TX (Outer Beam)	3
WS/TX Ratio when WS is at RX (Inner Beam)	4
WS/TX Ratio when WS is at RX (Outer Beam)	5
RX/TX Ratio (Inner Beam)	6
RX/TX Ratio (Outer Beam)	8
Optical Efficiency of Inner Beam	9
Optical Efficiency of Outer Beam	10
Total Optical Efficiency	11
TX/WS Ratio	12
RX/WS Ratio	14
TX/WS Ratio (Corrected for OE)	15
RX/WS Ratio (Corrected for OE)	16
Power Imbalance	17
Summary	18

About

This document contains the Pcal PD (TxPD and RxPD) Calibration trends. The first six sections contain the six ratios measured at the end-station labeled as m1, m2m6. The section that follows contains the relevant information calculated from these measurements which include Optical Efficiency, Power Imbalance, TX/WS and RX/WS ratio.

Understanding Each Section

Each section contains a list of measurements with Magnitude, Standard Error (Std Err) and Relative Error (Rel Err) for each measurement. The list is followed by two plot figures with Magnitude on the first plot and the the Normalized Magnitude on the second. Each section ends with a summary that contains the weighted mean of all the measurement along with their Standard Deviation (Std Dev), Std Err and Rel Err where each of


```
Mean = sum(x(i)*w(i))/sum(w(i))
Std Dev = sqrt(sum(w(i)*(x(i)-x_mean)^2)/((n-1)/n*sum(w(i))))
Std Err = Std Dev/sqrt(n)
Rel Err = Std Err/Mean
```

Report created on 31-Oct-2016

WS/TX Ratio when WS is at TX (Inner Beam)

List of Measurements

<i>Date</i>	<i>m1 ± SE_{m1}</i>	<i>Normalized</i>
D20150811	-0.180846 ± 0.000008	(1 ± 0.000044)
D20150827	-0.180614 ± 0.000007	(1 ± 0.000037)
D20151013	-0.180474 ± 0.000006	(1 ± 0.000034)
D20151222	-0.180696 ± 0.000008	(1 ± 0.000044)
D20160505	-0.178817 ± 0.000008	(1 ± 0.000043)
D20160628	-0.178884 ± 0.000007	(1 ± 0.000041)
D20160927	-0.179158 ± 0.000008	(1 ± 0.000046)
D20161011	-0.179883 ± 0.000010	(1 ± 0.000054)
D20161031	-0.181175 ± 0.000007	(1 ± 0.000040)

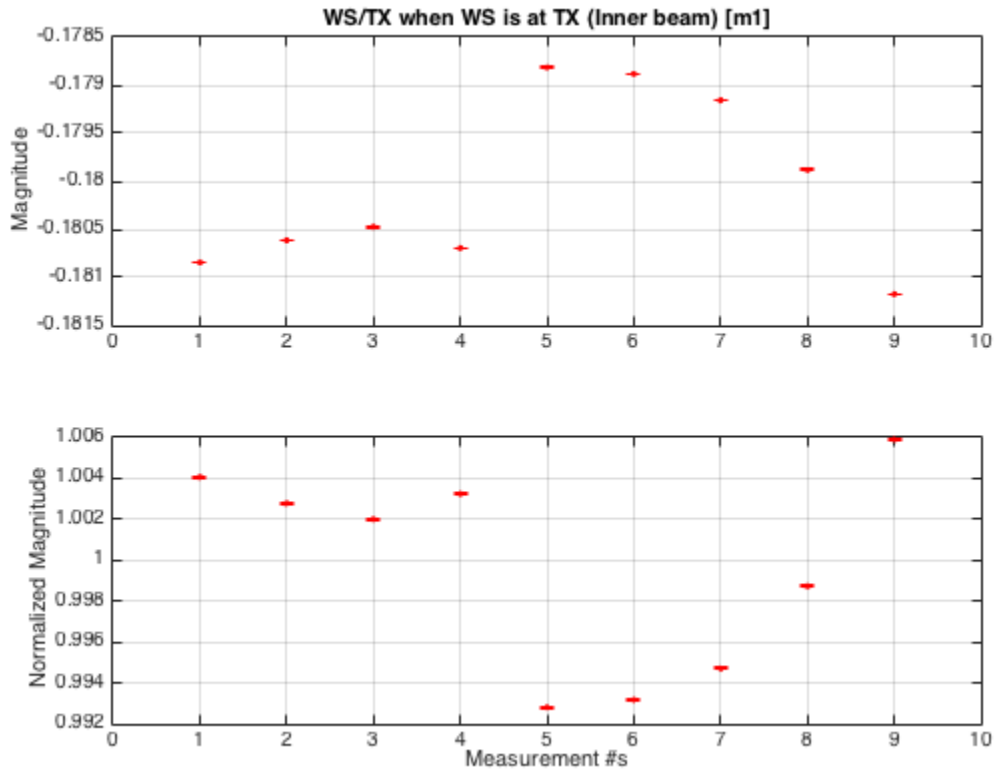


Summary of WS/TX when WS is at TX (Inner beam) [m1]:

Mean value: -0.180112
Standard deviation: 0.000897
Standard Error: 0.000317
Relative Standard Error: 0.001758

WS/TX Ratio when WS is at TX (Outer Beam)

List of Measurements

<i>Date</i>	<i>m2 ± SE_{m2}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-0.183815 ± 0.000007</i>	<i>(1 ± 0.000039)</i>
<i>D20150827</i>	<i>-0.183788 ± 0.000006</i>	<i>(1 ± 0.000035)</i>
<i>D20151013</i>	<i>-0.184127 ± 0.000007</i>	<i>(1 ± 0.000036)</i>
<i>D20151222</i>	<i>-0.184502 ± 0.000005</i>	<i>(1 ± 0.000027)</i>
<i>D20160505</i>	<i>-0.183087 ± 0.000008</i>	<i>(1 ± 0.000044)</i>
<i>D20160628</i>	<i>-0.183461 ± 0.000008</i>	<i>(1 ± 0.000042)</i>
<i>D20160927</i>	<i>-0.184007 ± 0.000008</i>	<i>(1 ± 0.000044)</i>
<i>D20161011</i>	<i>-0.181887 ± 0.000010</i>	<i>(1 ± 0.000053)</i>
<i>D20161031</i>	<i>-0.183163 ± 0.000008</i>	<i>(1 ± 0.000041)</i>

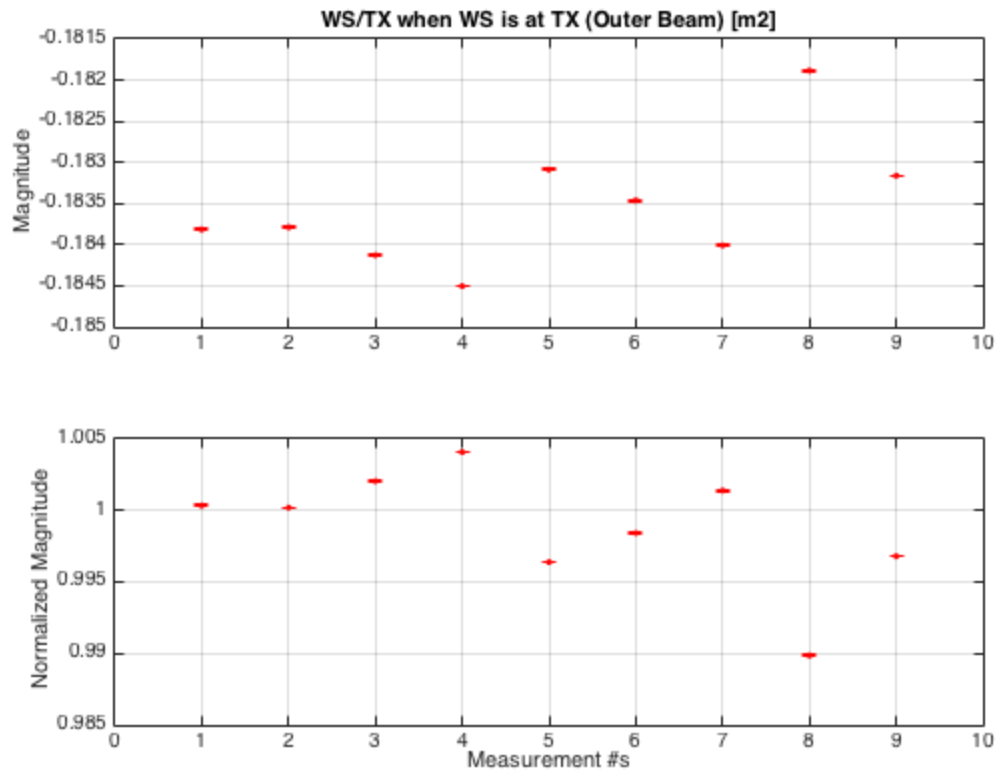


Summary of WS/TX when WS is at TX (Outer Beam) [m2]:
Mean value: -0.183751
Standard deviation: 0.000698
Standard Error: 0.000246
Relative Standard Error: 0.001341

WS/TX Ratio when WS is at RX (Inner Beam)

List of Measurements

Date	$m3 \pm SE_{\{m3\}}$	Normalized
D20150811	-0.179002 $\pm$ 0.000008	(1 $\pm$ 0.000043)
D20150827	-0.176861 $\pm$ 0.000006	(1 $\pm$ 0.000036)
D20151013	-0.178931 $\pm$ 0.000006	(1 $\pm$ 0.000035)
D20151222	-0.179098 $\pm$ 0.000007	(1 $\pm$ 0.000037)
D20160505	-0.177402 $\pm$ 0.000008	(1 $\pm$ 0.000043)
D20160628	-0.177210 $\pm$ 0.000008	(1 $\pm$ 0.000043)
D20160927	-0.178050 $\pm$ 0.000008	(1 $\pm$ 0.000046)

<i>D20161011</i>	-0.177663 ± 0.000009	(1 ± 0.000050)
<i>D20161031</i>	-0.179651 ± 0.000008	(1 ± 0.000044)

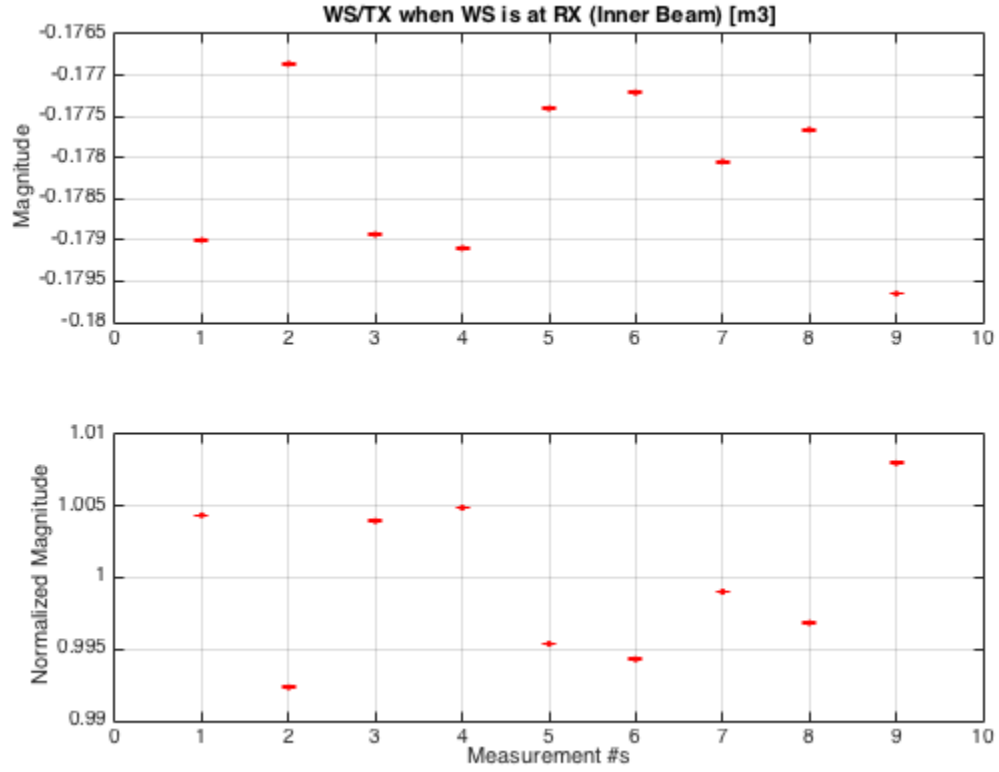


Summary of WS/TX when WS is at RX (Inner Beam) [m3]:
Mean value: -0.178225
Standard deviation: 0.001008
Standard Error: 0.000356
Relative Standard Error: 0.001997

WS/TX Ratio when WS is at RX (Outer Beam)

List of Measurements

<i>Date</i>	$m4 \pm SE_{\{m4\}}$	<i>Normalized</i>
<i>D20150811</i>	-0.181381 ± 0.000008	(1 ± 0.000046)
<i>D20150827</i>	-0.181640 ± 0.000006	(1 ± 0.000031)
<i>D20151013</i>	-0.181781 ± 0.000006	(1 ± 0.000034)
<i>D20151222</i>	-0.182083 ± 0.000006	(1 ± 0.000031)

D20160505	-0.180668 ± 0.000007	(1 ± 0.000040)
D20160628	-0.180940 ± 0.000007	(1 ± 0.000040)
D20160927	-0.182118 ± 0.000009	(1 ± 0.000048)
D20161011	-0.179869 ± 0.000008	(1 ± 0.000046)
D20161031	-0.180443 ± 0.000008	(1 ± 0.000045)

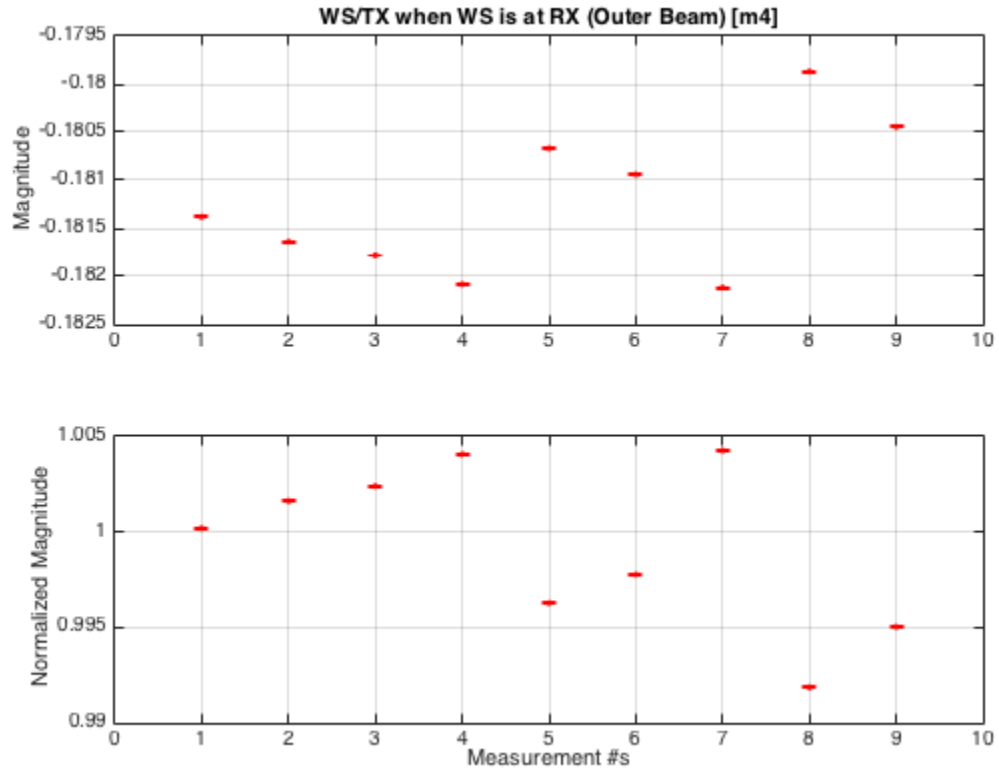

Summary of WS/TX when WS is at RX (Outer Beam) [m4]:

Mean value:	-0.181345
Standard deviation:	0.000732
Standard Error:	0.000258
Relative Standard Error:	0.001424


RX/TX Ratio (Inner Beam)

List of Measurements

Date	$m5 \pm SE_{\{m5\}}$	Normalized
D20150811	0.716408 ± 0.000003	(1 ± 0.000005)

LHOY-End RxPD and Tx-
PD Calibration Trends

D20150827	0.715858 ± 0.000003	(1 ± 0.000004)
D20151013	0.715399 ± 0.000002	(1 ± 0.000003)
D20151222	0.716771 ± 0.000002	(1 ± 0.000003)
D20160505	0.717343 ± 0.000002	(1 ± 0.000003)
D20160628	0.715799 ± 0.000002	(1 ± 0.000003)
D20160927	0.715156 ± 0.000003	(1 ± 0.000004)
D20161011	0.715926 ± 0.000004	(1 ± 0.000006)
D20161031	0.721892 ± 0.000003	(1 ± 0.000004)

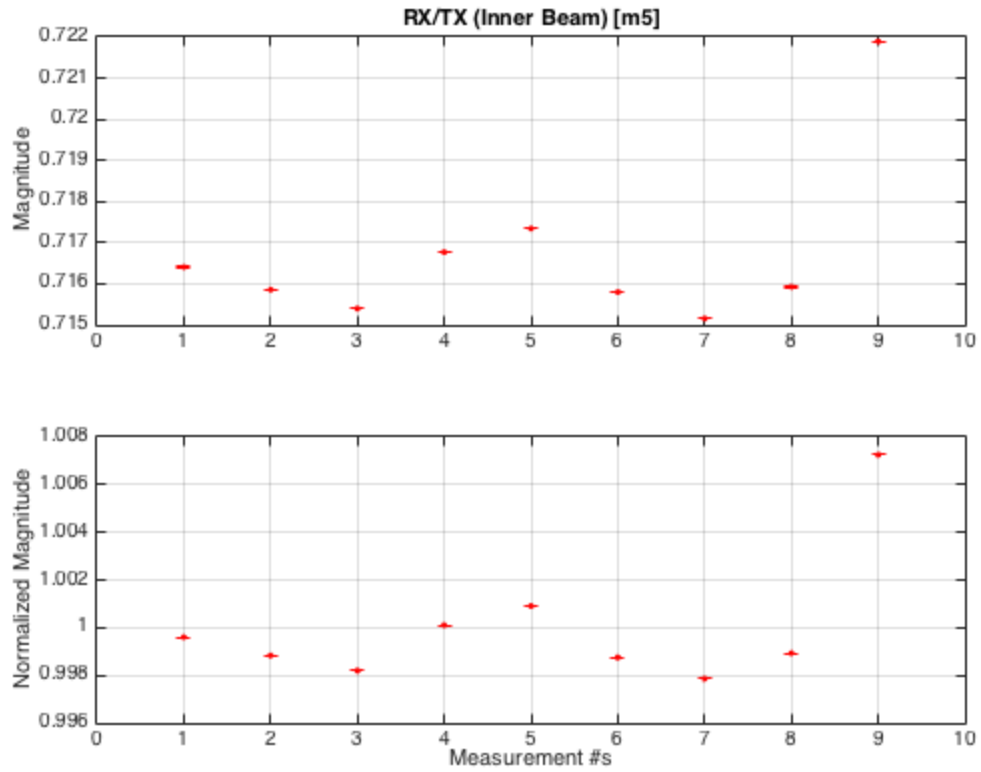


Summary of RX/TX (Inner Beam) [m5]:

Mean value: 0.716695
 Standard deviation: 0.001923
 Standard Error: 0.000679
 Relative Standard Error: 0.000947

RX/TX Ratio (Outer Beam)

List of Measurements

<i>Date</i>	<i>m6 ± SE_{m6}</i>	<i>Normalized</i>
D20150811	0.726657 ± 0.000003	(1 ± 0.000004)
D20150827	0.726468 ± 0.000002	(1 ± 0.000003)
D20151013	0.727582 ± 0.000002	(1 ± 0.000003)
D20151222	0.728972 ± 0.000002	(1 ± 0.000003)
D20160505	0.730960 ± 0.000002	(1 ± 0.000003)
D20160628	0.732089 ± 0.000003	(1 ± 0.000004)
D20160927	0.732393 ± 0.000002	(1 ± 0.000003)
D20161011	0.726292 ± 0.000003	(1 ± 0.000004)
D20161031	0.725420 ± 0.000002	(1 ± 0.000003)

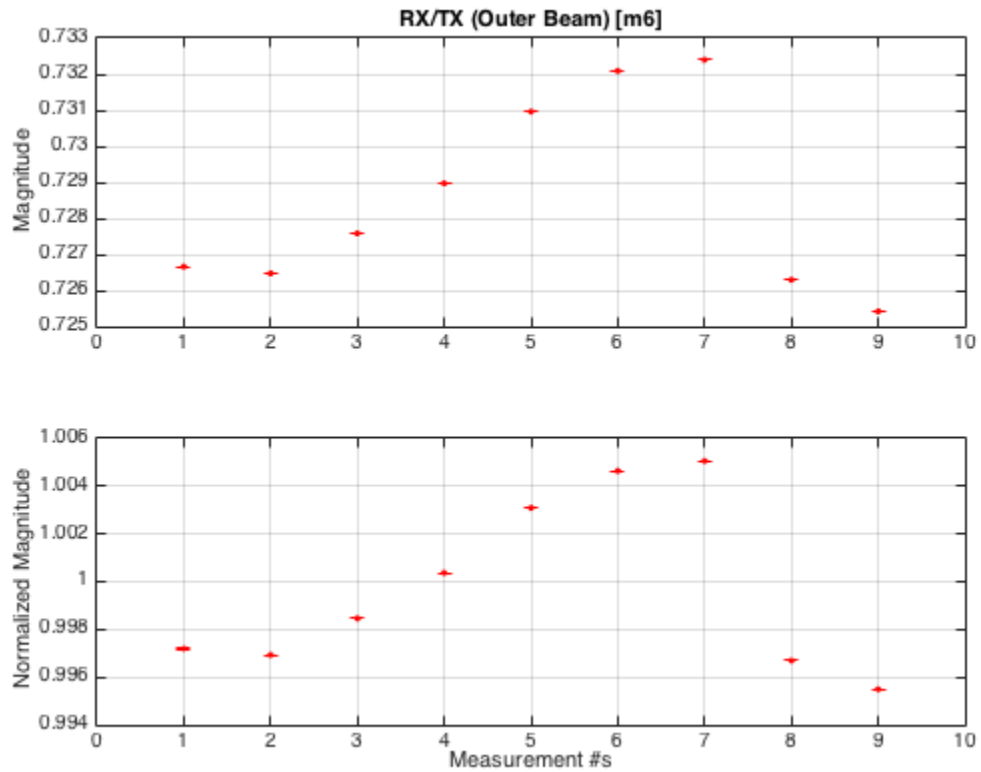


Summary of RX/TX (Outer Beam) [m6]:

Mean value: 0.728704
Standard deviation: 0.002577
Standard Error: 0.000909
Relative Standard Error: 0.001248

Optical Efficiency of Inner Beam

List of Measurements

<i>Date</i>	<i>$e_i \pm SE_{\{e_i\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>0.989808 ± 0.000062</i>	<i>(1 ± 0.000062)</i>
<i>D20150827</i>	<i>0.979224 ± 0.000052</i>	<i>(1 ± 0.000053)</i>
<i>D20151013</i>	<i>0.991448 ± 0.000049</i>	<i>(1 ± 0.000049)</i>
<i>D20151222</i>	<i>0.991154 ± 0.000057</i>	<i>(1 ± 0.000058)</i>
<i>D20160505</i>	<i>0.992086 ± 0.000061</i>	<i>(1 ± 0.000061)</i>
<i>D20160628</i>	<i>0.990643 ± 0.000059</i>	<i>(1 ± 0.000060)</i>
<i>D20160927</i>	<i>0.993815 ± 0.000065</i>	<i>(1 ± 0.000065)</i>
<i>D20161011</i>	<i>0.987658 ± 0.000074</i>	<i>(1 ± 0.000075)</i>
<i>D20161031</i>	<i>0.991589 ± 0.000060</i>	<i>(1 ± 0.000060)</i>

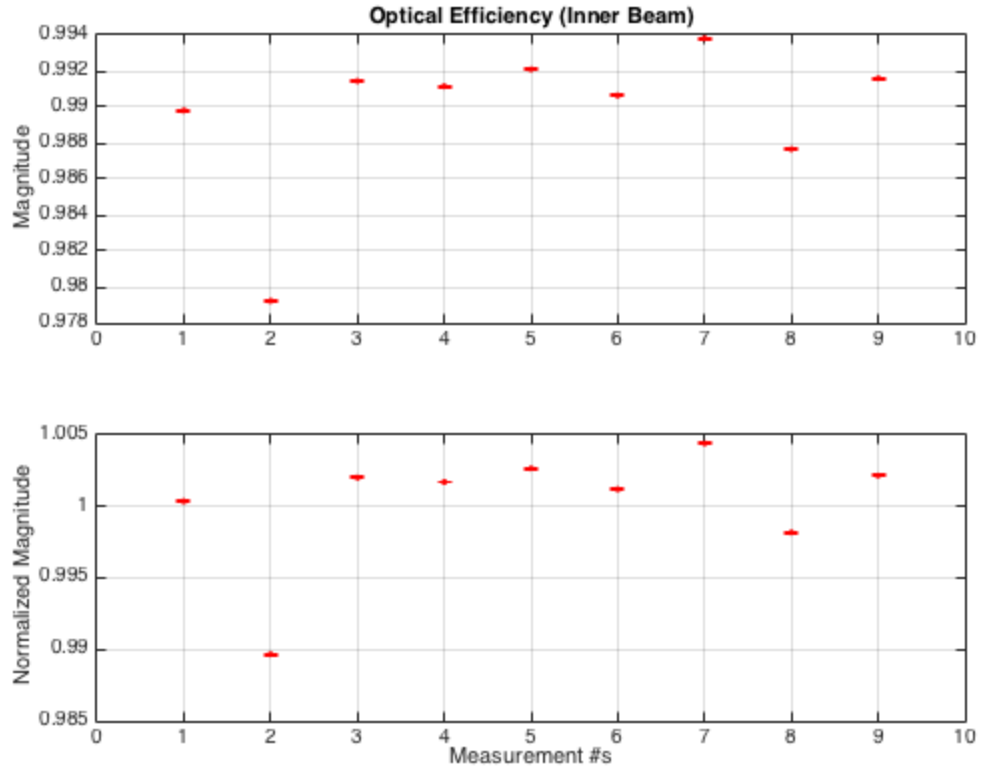

Summary of Optical Efficiency (Inner Beam):


Mean value: 0.989452
Standard deviation: 0.004646
Standard Error: 0.001640
Relative Standard Error: 0.001657

Optical Efficiency of Outer Beam

List of Measurements

Date	$e_o \pm SE_{\{e_o\}}$	Normalized
D20150811	0.986759 ± 0.000061	(1 ± 0.000062)
D20150827	0.988317 ± 0.000047	(1 ± 0.000047)
D20151013	0.987256 ± 0.000049	(1 ± 0.000050)
D20151222	0.986890 ± 0.000041	(1 ± 0.000041)
D20160505	0.986788 ± 0.000060	(1 ± 0.000061)
D20160628	0.986257 ± 0.000058	(1 ± 0.000059)
D20160927	0.989731 ± 0.000065	(1 ± 0.000066)

<i>D20161011</i>	<i>0.988909 ± 0.000070</i>	<i>(1 ± 0.000071)</i>
<i>D20161031</i>	<i>0.985153 ± 0.000061</i>	<i>(1 ± 0.000062)</i>

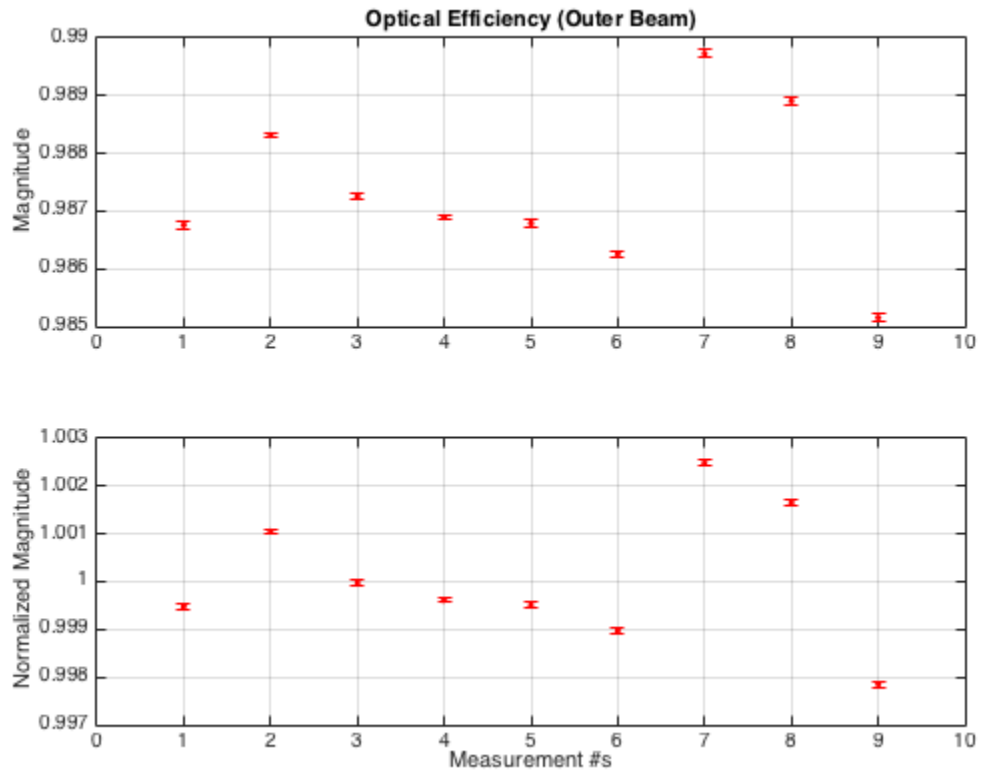

Summary of Optical Efficiency (Outer Beam):


<i>Mean value:</i>	<i>0.987274</i>
<i>Standard deviation:</i>	<i>0.001248</i>
<i>Standard Error:</i>	<i>0.000440</i>
<i>Relative Standard Error:</i>	<i>0.000446</i>

Total Optical Efficiency

List of Measurements

<i>Date</i>	<i>e ± SE_{e}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>0.988271 ± 0.000043</i>	<i>(1 ± 0.000043)</i>
<i>D20150827</i>	<i>0.983810 ± 0.000034</i>	<i>(1 ± 0.000035)</i>
<i>D20151013</i>	<i>0.989331 ± 0.000034</i>	<i>(1 ± 0.000035)</i>
<i>D20151222</i>	<i>0.989000 ± 0.000035</i>	<i>(1 ± 0.000035)</i>

<i>D20160505</i>	<i>0.989405 ± 0.000042</i>	<i>(1 ± 0.000043)</i>
<i>D20160628</i>	<i>0.988423 ± 0.000041</i>	<i>(1 ± 0.000041)</i>
<i>D20160927</i>	<i>0.991746 ± 0.000046</i>	<i>(1 ± 0.000046)</i>
<i>D20161011</i>	<i>0.988287 ± 0.000050</i>	<i>(1 ± 0.000051)</i>
<i>D20161031</i>	<i>0.988353 ± 0.000042</i>	<i>(1 ± 0.000043)</i>

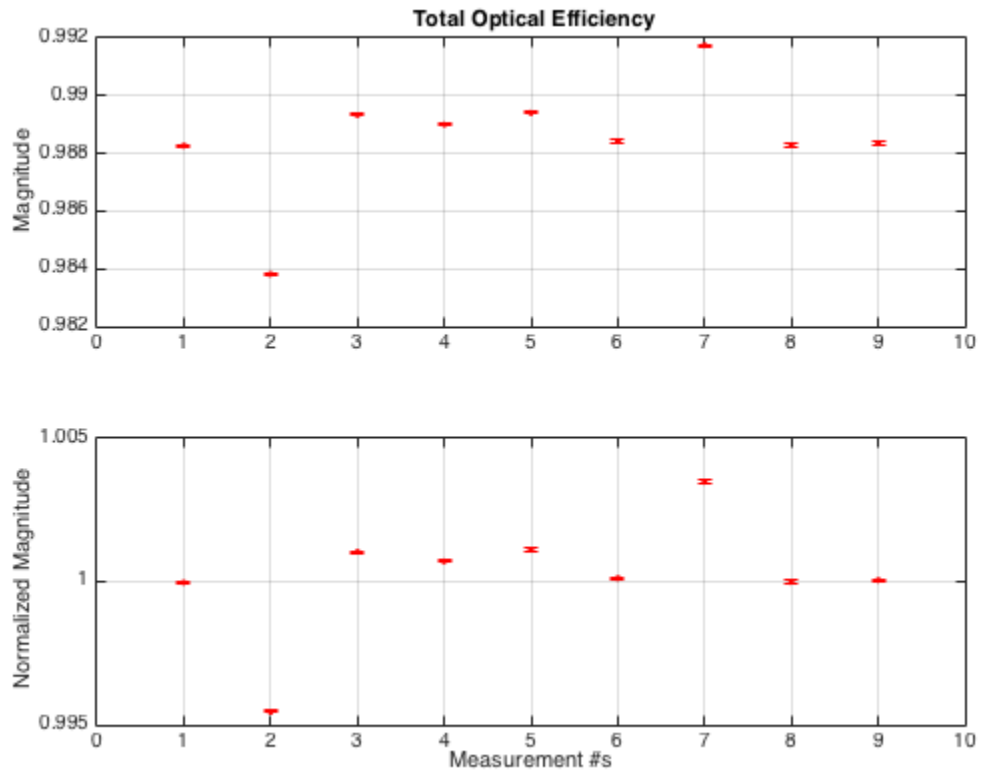

Summary of Total Optical Efficiency:

<i>Mean value:</i>	<i>0.988300</i>
<i>Standard deviation:</i>	<i>0.002221</i>
<i>Standard Error:</i>	<i>0.000784</i>
<i>Relative Standard Error:</i>	<i>0.000793</i>


TX/WS Ratio

List of Measurements

<i>Date</i>	<i>R_TW ± SE_{R_TW}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-2.742279 ± 0.000011</i>	<i>(1 ± 0.000004)</i>

LHOY-End RxPD and Tx-
PD Calibration Trends

D20150827	-2.744228 ± 0.000009	(1 ± 0.000003)
D20151013	-2.742723 ± 0.000009	(1 ± 0.000003)
D20151222	-2.738239 ± 0.000009	(1 ± 0.000003)
D20160505	-2.763161 ± 0.000011	(1 ± 0.000004)
D20160628	-2.759803 ± 0.000011	(1 ± 0.000004)
D20160927	-2.753569 ± 0.000011	(1 ± 0.000004)
D20161011	-2.764191 ± 0.000014	(1 ± 0.000005)
D20161031	-2.744705 ± 0.000010	(1 ± 0.000004)

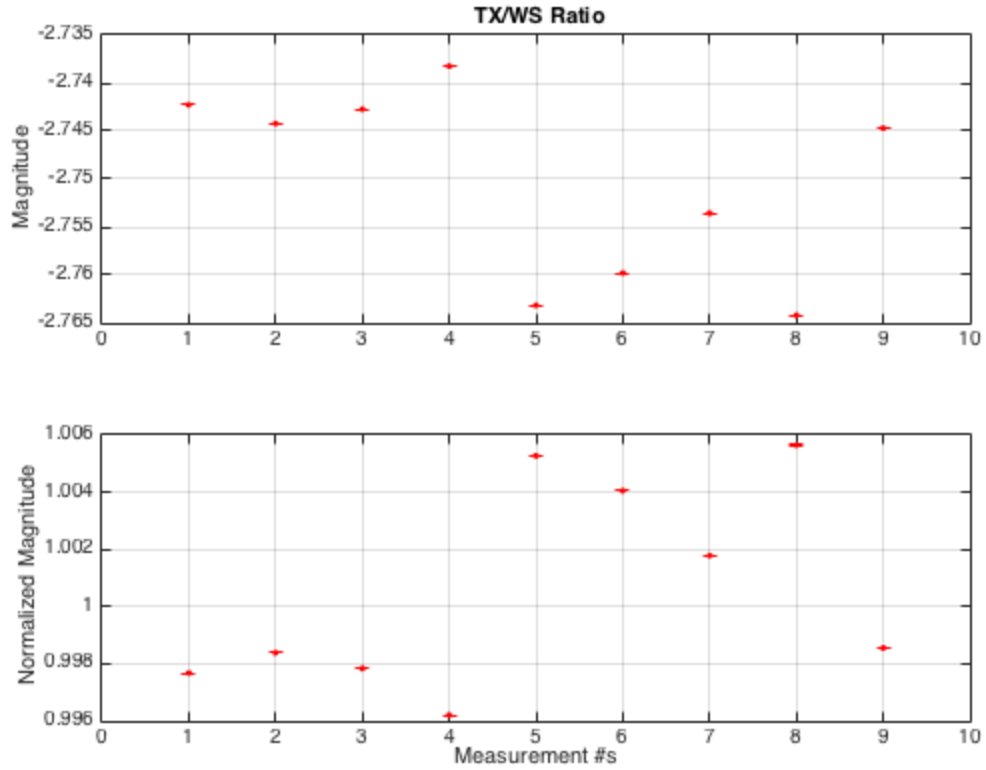


Summary of TX/WS Ratio:

Mean value:	-2.748673
Standard deviation:	0.009507
Standard Error:	0.003355
Relative Standard Error:	0.001221

RX/WS Ratio

List of Measurements

<i>Date</i>	<i>$R_{RW} \pm SE_{\{R_{RW}\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-4.004239 ± 0.000126</i>	<i>(1 ± 0.000032)</i>
<i>D20150827</i>	<i>-4.023526 ± 0.000096</i>	<i>(1 ± 0.000024)</i>
<i>D20151013</i>	<i>-4.000359 ± 0.000097</i>	<i>(1 ± 0.000024)</i>
<i>D20151222</i>	<i>-4.002816 ± 0.000096</i>	<i>(1 ± 0.000024)</i>
<i>D20160505</i>	<i>-4.044736 ± 0.000119</i>	<i>(1 ± 0.000029)</i>
<i>D20160628</i>	<i>-4.042655 ± 0.000118</i>	<i>(1 ± 0.000029)</i>
<i>D20160927</i>	<i>-4.019073 ± 0.000135</i>	<i>(1 ± 0.000033)</i>
<i>D20161011</i>	<i>-4.033790 ± 0.000139</i>	<i>(1 ± 0.000034)</i>
<i>D20161031</i>	<i>-4.019253 ± 0.000127</i>	<i>(1 ± 0.000032)</i>

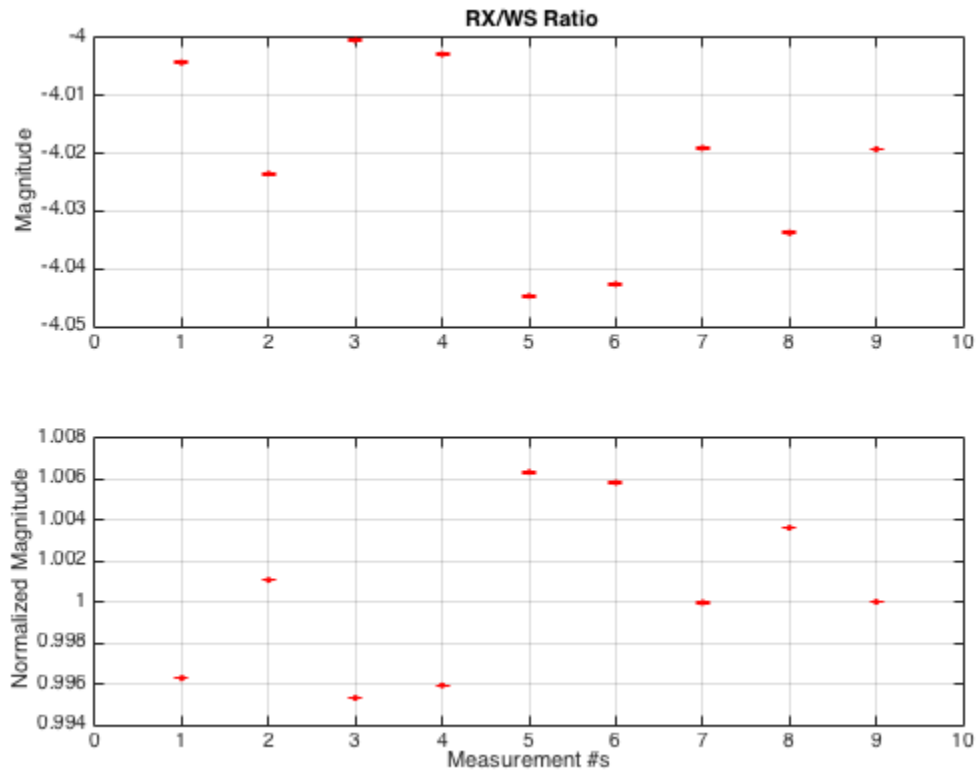


Summary of RX/WS Ratio:

Mean value: -4.019174
Standard deviation: 0.017024
Standard Error: 0.006008
Relative Standard Error: 0.001495

TX/WS Ratio (Corrected for OE)

List of Measurements

<i>Date</i>	<i>R_Twc ± SE_{R_Twc}</i>	<i>Normalized</i>
D20150811	-2.758456 ± 0.000060	(1 ± 0.000022)
D20150827	-2.766624 ± 0.000048	(1 ± 0.000017)
D20151013	-2.757433 ± 0.000048	(1 ± 0.000017)
D20151222	-2.753383 ± 0.000048	(1 ± 0.000018)
D20160505	-2.777877 ± 0.000059	(1 ± 0.000021)
D20160628	-2.775872 ± 0.000058	(1 ± 0.000021)
D20160927	-2.764980 ± 0.000064	(1 ± 0.000023)
D20161011	-2.780474 ± 0.000071	(1 ± 0.000025)
D20161031	-2.760782 ± 0.000059	(1 ± 0.000021)

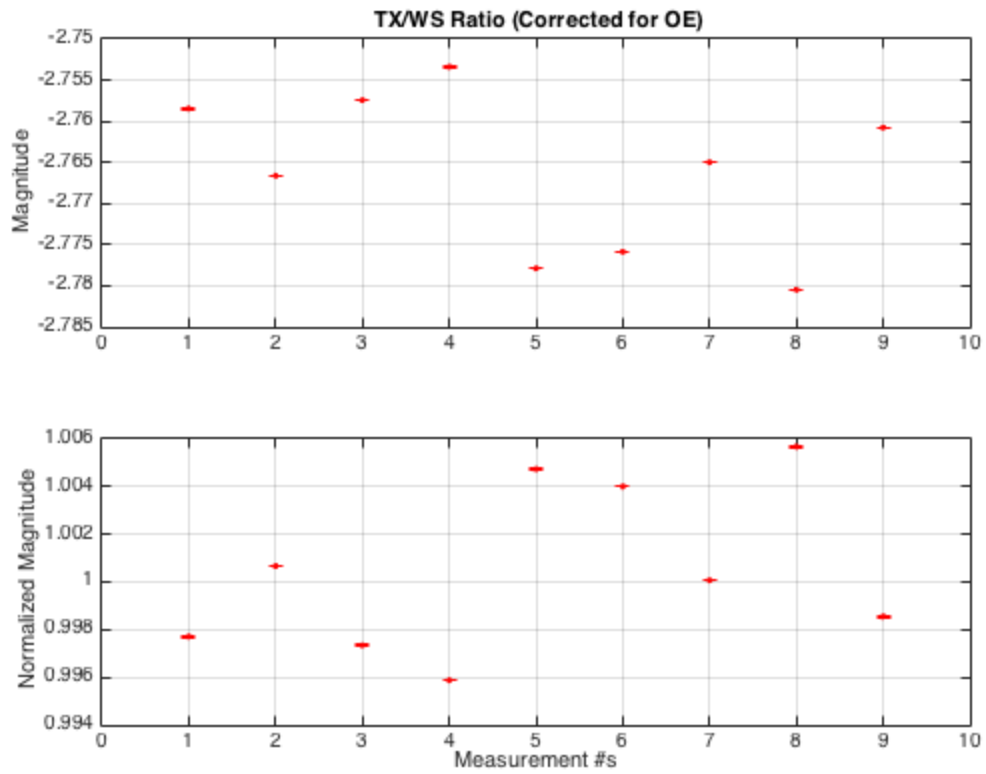

Summary of TX/WS Ratio (Corrected for OE):


Mean value: -2.764784
Standard deviation: 0.009482
Standard Error: 0.003346
Relative Standard Error: 0.001210

RX/WS Ratio (Corrected for OE)

List of Measurements

Date	$R_{Rwc} \pm SE_{\{R_{Rwc}\}}$	Normalized
D20150811	-3.980617 ± 0.000087	(1 ± 0.000022)
D20150827	-3.990691 ± 0.000070	(1 ± 0.000018)
D20151013	-3.978905 ± 0.000069	(1 ± 0.000017)
D20151222	-3.980678 ± 0.000070	(1 ± 0.000018)
D20160505	-4.023196 ± 0.000086	(1 ± 0.000021)
D20160628	-4.019117 ± 0.000084	(1 ± 0.000021)
D20160927	-4.002417 ± 0.000092	(1 ± 0.000023)

D20161011	-4.010027 ± 0.000103	(1 ± 0.000026)
D20161031	-3.995710 ± 0.000086	(1 ± 0.000022)

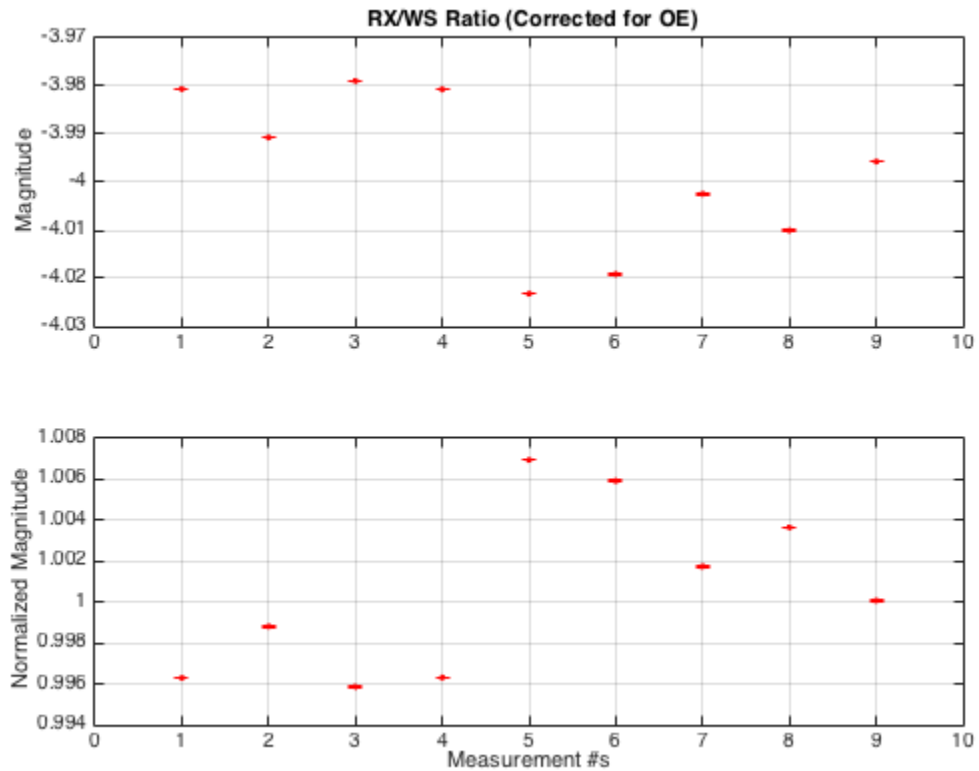

Summary of RX/WS Ratio (Corrected for OE):


Mean value:	-3.995427
Standard deviation:	0.016813
Standard Error:	0.005934
Relative Standard Error:	0.001485

Power Imbalance

List of Measurements

D20150811	0.983938 ± 0.000059	(1 ± 0.000059)
D20150827	0.982844 ± 0.000050	(1 ± 0.000051)
D20151013	0.980135 ± 0.000048	(1 ± 0.000049)
D20151222	0.979459 ± 0.000051	(1 ± 0.000052)
D20160505	0.976585 ± 0.000060	(1 ± 0.000062)

D20160628	0.974999 ± 0.000057	(1 ± 0.000059)
D20160927	0.973728 ± 0.000061	(1 ± 0.000063)
D20161011	0.989087 ± 0.000075	(1 ± 0.000075)
D20161031	0.989175 ± 0.000057	(1 ± 0.000058)

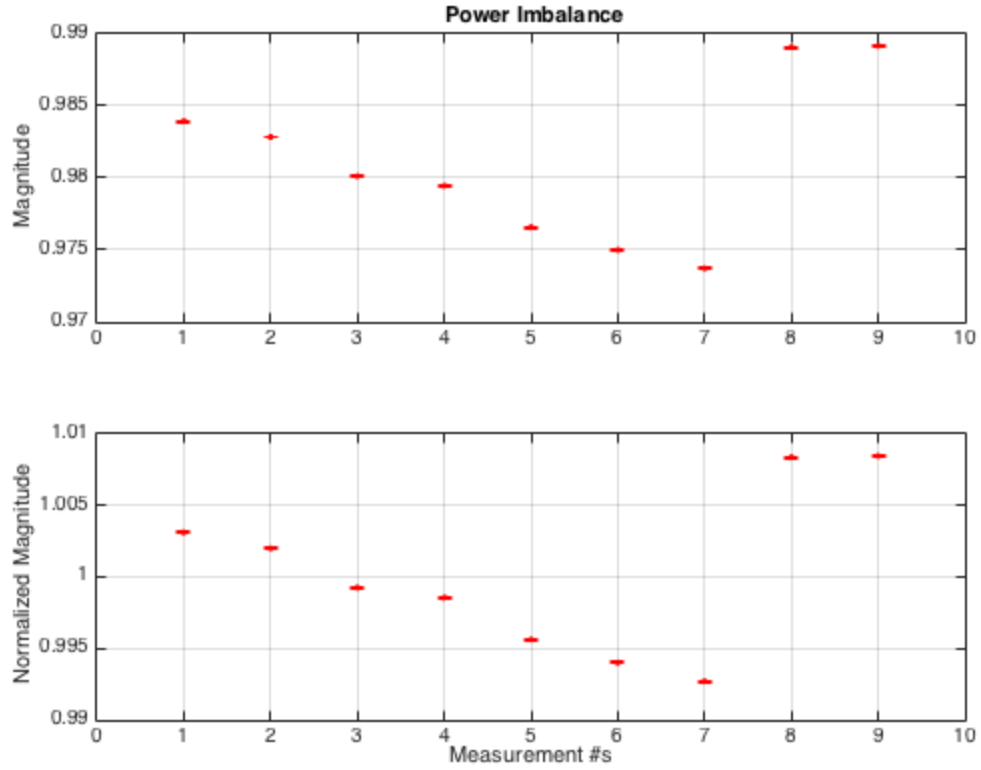

Summary of Power Imbalance:

Mean value:	0.980877
Standard deviation:	0.005179
Standard Error:	0.001828
Relative Standard Error:	0.001863

Summary

Description	Value	Std Dev	Std Err	Rel Err:
OE (e)	0.9883	0.0022	0.0008	0.0008
TX/WS (a1a2)	-2.7648	0.0095	0.0033	0.0012
RX/WS (b1b2)	-3.9954	0.0168	0.0059	0.0015
W (a5)	1.0000	----	----	0.0034

Published with MATLAB® R2014b