
LHOY-End RxPD and TxPD Calibration Trends

Table of Contents

About	1
WS/TX Ratio when WS is at TX (Inner Beam)	2
WS/TX Ratio when WS is at TX (Outer Beam)	3
WS/TX Ratio when WS is at RX (Inner Beam)	4
WS/TX Ratio when WS is at RX (Outer Beam)	6
RX/TX Ratio (Inner Beam)	7
RX/TX Ratio (Outer Beam)	8
Optical Efficiency of Inner Beam	10
Optical Efficiency of Outer Beam	11
Total Optical Efficiency	12
TX/WS Ratio	14
RX/WS Ratio	15
TX/WS Ratio (Corrected for OE)	16
RX/WS Ratio (Corrected for OE)	18
Power Imbalance	19
Summary	20

About

This document contains the Pcal PD (TxPD and RxPD) Calibration trends. The first six sections contain the six ratios measured at the end-station labeled as m1, m2m6. The section that follows contains the relevant information calculated from these measurements which include Optical Efficiency, Power Imbalance, TX/WS and RX/WS ratio.

Understanding Each Section

Each section contains a list of measurements with Magnitude, Standard Error (Std Err) and Relative Error (Rel Err) for each measurement. The list is followed by two plot figures with Magnitude on the first plot and the the Normalized Magnitude on the second. Each section ends with a summary that contains the weighted mean of all the measurement along with their Standard Deviation (Std Dev), Std Err and Rel Err where each of


$$\begin{aligned} \text{Mean} &= \text{sum}(x(i)*w(i))/\text{sum}(w(i)) \\ \text{Std Dev} &= \text{sqr}t(\text{sum}(w(i)*(x(i)-x_mean)^2)/((n-1)/n*\text{sum}(w(i)))) \\ \text{Std Err} &= \text{Std Dev}/\text{sqr}t(n) \\ \text{Rel Err} &= \text{Std Err}/\text{Mean} \end{aligned}$$

Report created on 17-Jan-2017

WS/TX Ratio when WS is at TX (Inner Beam)

List of Measurements

<i>Date</i>	<i>$m1 \pm SE_{\{m1\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-0.180846 ± 0.000008</i>	<i>(1 ± 0.000044)</i>
<i>D20150827</i>	<i>-0.180614 ± 0.000007</i>	<i>(1 ± 0.000037)</i>
<i>D20151013</i>	<i>-0.180474 ± 0.000006</i>	<i>(1 ± 0.000034)</i>
<i>D20151222</i>	<i>-0.180696 ± 0.000008</i>	<i>(1 ± 0.000044)</i>
<i>D20160505</i>	<i>-0.178817 ± 0.000008</i>	<i>(1 ± 0.000043)</i>
<i>D20160628</i>	<i>-0.178884 ± 0.000007</i>	<i>(1 ± 0.000041)</i>
<i>D20160927</i>	<i>-0.179158 ± 0.000008</i>	<i>(1 ± 0.000046)</i>
<i>D20161011</i>	<i>-0.179883 ± 0.000010</i>	<i>(1 ± 0.000054)</i>
<i>D20161031</i>	<i>-0.181175 ± 0.000007</i>	<i>(1 ± 0.000040)</i>
<i>D20161109</i>	<i>-0.162027 ± 0.000016</i>	<i>(1 ± 0.000102)</i>
<i>D20170117</i>	<i>-0.161686 ± 0.000024</i>	<i>(1 ± 0.000146)</i>

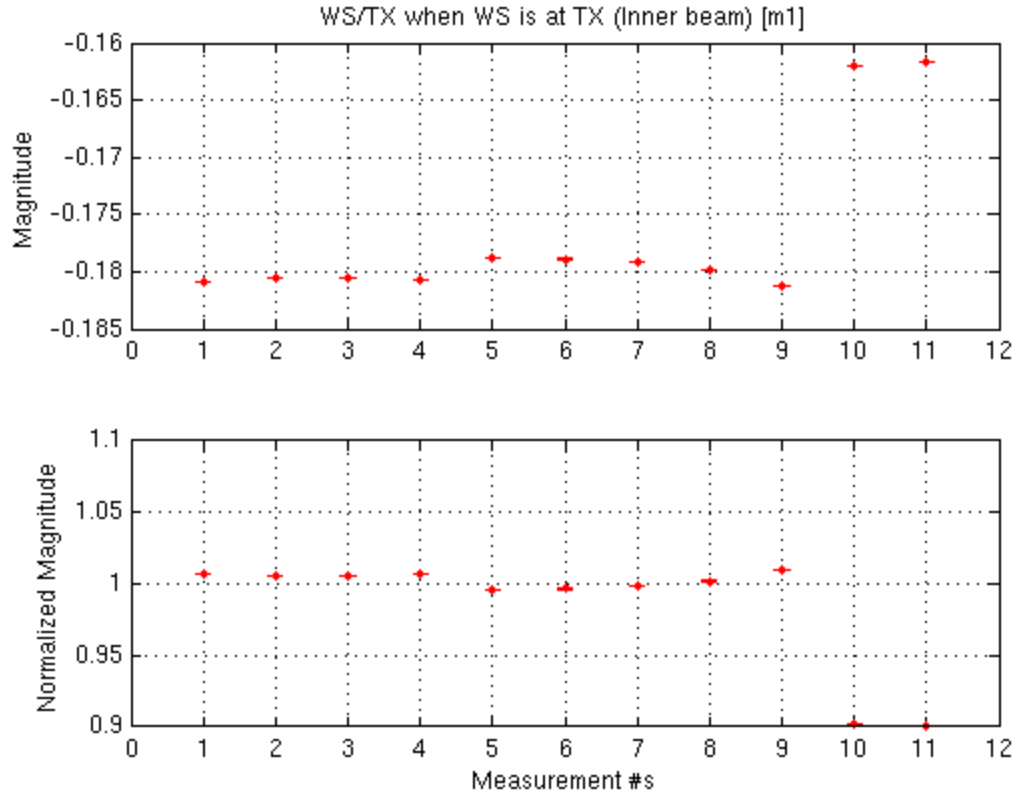


Summary of WS/TX when WS is at TX (Inner beam) [m1]:
Mean value: -0.179508
Standard deviation: 0.003529
Standard Error: 0.001115
Relative Standard Error: 0.006210

WS/TX Ratio when WS is at TX (Outer Beam)

List of Measurements

Date	$m2 \pm SE_{\{m2\}}$	Normalized
D20150811	-0.183815 ± 0.000007	(1 ± 0.000039)
D20150827	-0.183788 ± 0.000006	(1 ± 0.000035)
D20151013	-0.184127 ± 0.000007	(1 ± 0.000036)
D20151222	-0.184502 ± 0.000005	(1 ± 0.000027)
D20160505	-0.183087 ± 0.000008	(1 ± 0.000044)
D20160628	-0.183461 ± 0.000008	(1 ± 0.000042)
D20160927	-0.184007 ± 0.000008	(1 ± 0.000044)

<i>D20161011</i>	-0.181887 ± 0.000010	(1 ± 0.000053)
<i>D20161031</i>	-0.183163 ± 0.000008	(1 ± 0.000041)
<i>D20161109</i>	-0.163651 ± 0.000015	(1 ± 0.000094)
<i>D20170117</i>	-0.165437 ± 0.000024	(1 ± 0.000142)

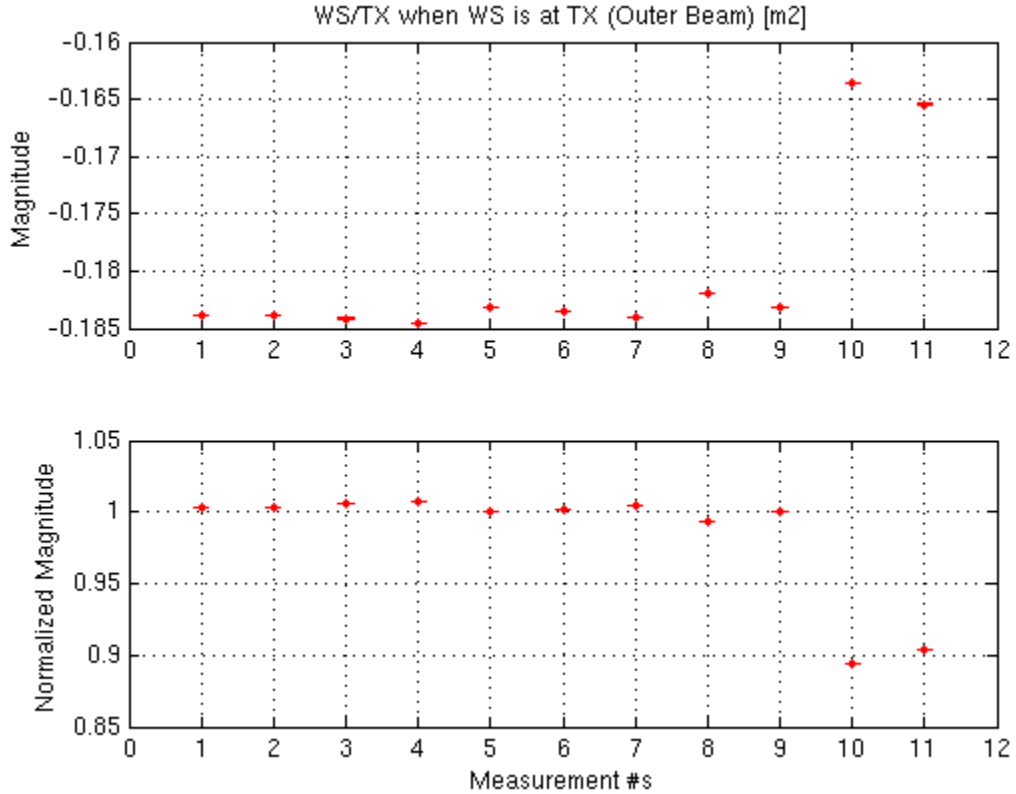


Summary of WS/TX when WS is at TX (Outer Beam) [m2]:
Mean value: -0.183124
Standard deviation: 0.003679
Standard Error: 0.001162
Relative Standard Error: 0.006346

WS/TX Ratio when WS is at RX (Inner Beam)

List of Measurements

<i>Date</i>	$m3 \pm SE_{\{m3\}}$	<i>Normalized</i>
<i>D20150811</i>	-0.179002 ± 0.000008	(1 ± 0.000043)
<i>D20150827</i>	-0.176861 ± 0.000006	(1 ± 0.000036)

D20151013	-0.178931 ± 0.000006	(1 ± 0.000035)
D20151222	-0.179098 ± 0.000007	(1 ± 0.000037)
D20160505	-0.177402 ± 0.000008	(1 ± 0.000043)
D20160628	-0.177210 ± 0.000008	(1 ± 0.000043)
D20160927	-0.178050 ± 0.000008	(1 ± 0.000046)
D20161011	-0.177663 ± 0.000009	(1 ± 0.000050)
D20161031	-0.179651 ± 0.000008	(1 ± 0.000044)
D20161109	-0.160833 ± 0.000019	(1 ± 0.000120)
D20170117	-0.157927 ± 0.000018	(1 ± 0.000114)

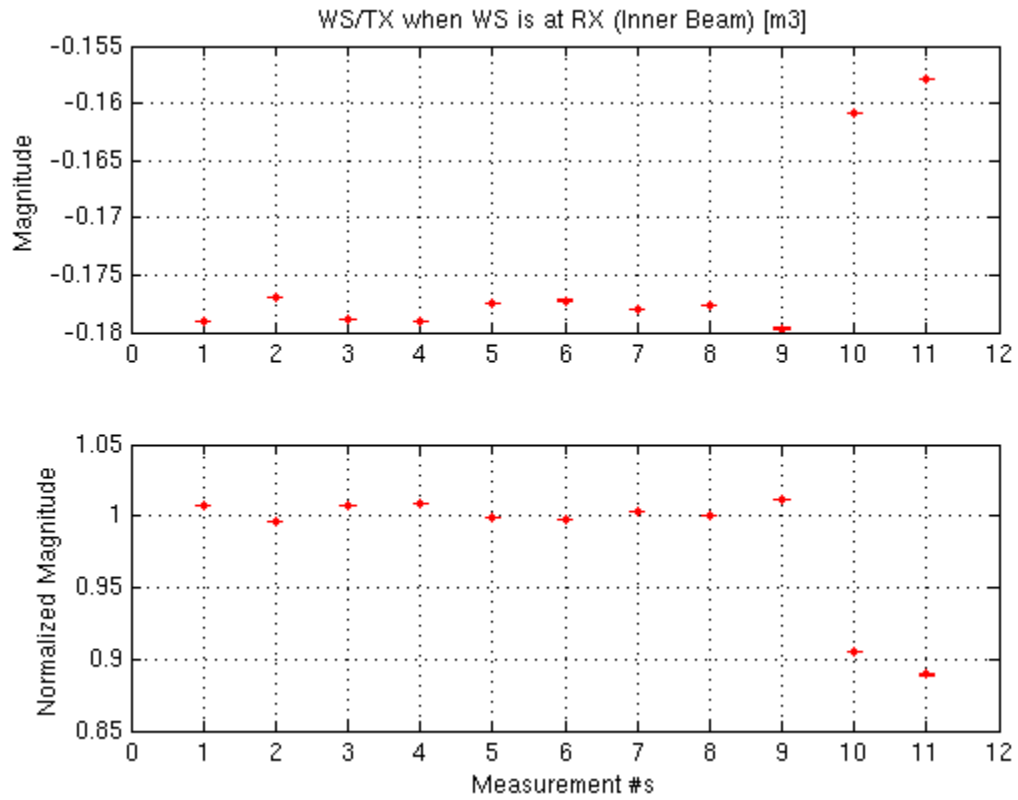


Summary of WS/TX when WS is at RX (Inner Beam) [m3]:

Mean value:	-0.177597
Standard deviation:	0.003702
Standard Error:	0.001169
Relative Standard Error:	0.006583

WS/TX Ratio when WS is at RX (Outer Beam)

List of Measurements

<i>Date</i>	<i>$m4 \pm SE_{\{m4\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-0.181381 ± 0.000008</i>	<i>(1 ± 0.000046)</i>
<i>D20150827</i>	<i>-0.181640 ± 0.000006</i>	<i>(1 ± 0.000031)</i>
<i>D20151013</i>	<i>-0.181781 ± 0.000006</i>	<i>(1 ± 0.000034)</i>
<i>D20151222</i>	<i>-0.182083 ± 0.000006</i>	<i>(1 ± 0.000031)</i>
<i>D20160505</i>	<i>-0.180668 ± 0.000007</i>	<i>(1 ± 0.000040)</i>
<i>D20160628</i>	<i>-0.180940 ± 0.000007</i>	<i>(1 ± 0.000040)</i>
<i>D20160927</i>	<i>-0.182118 ± 0.000009</i>	<i>(1 ± 0.000048)</i>
<i>D20161011</i>	<i>-0.179869 ± 0.000008</i>	<i>(1 ± 0.000046)</i>
<i>D20161031</i>	<i>-0.180443 ± 0.000008</i>	<i>(1 ± 0.000045)</i>
<i>D20161109</i>	<i>-0.161159 ± 0.000019</i>	<i>(1 ± 0.000118)</i>
<i>D20170117</i>	<i>-0.159364 ± 0.000157</i>	<i>(1 ± 0.000983)</i>

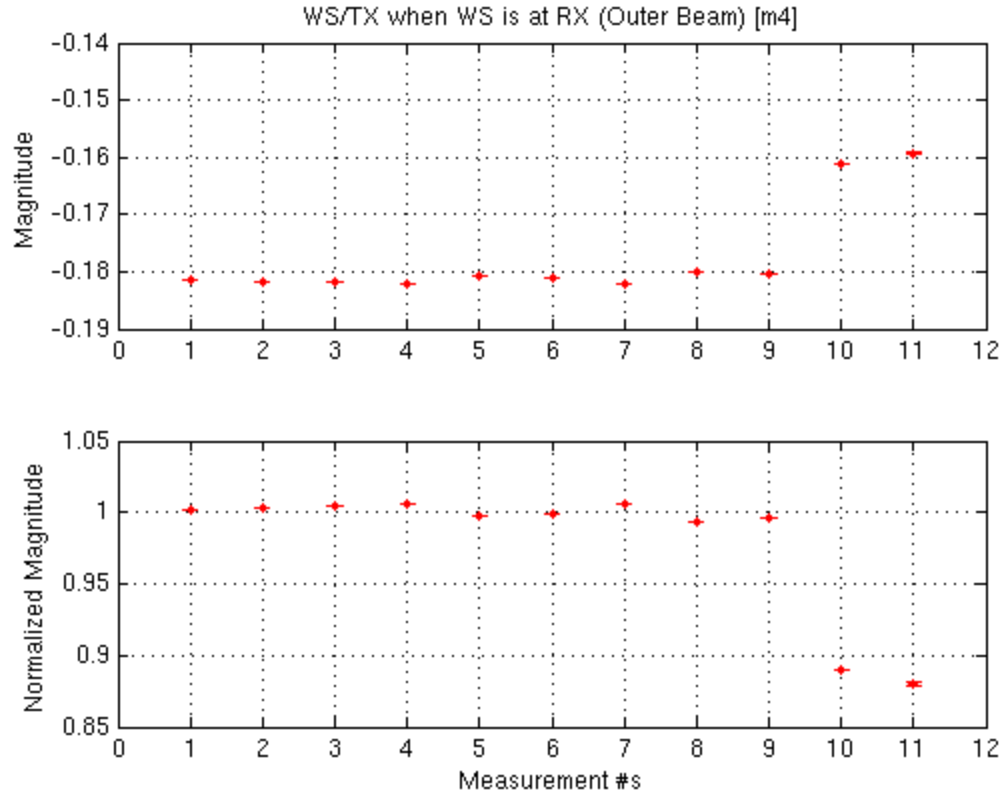

Summary of WS/TX when WS is at RX (Outer Beam) [m4]:


Mean value:	-0.181043
Standard deviation:	0.002671
Standard Error:	0.000844
Relative Standard Error:	0.004660

RX/TX Ratio (Inner Beam)

List of Measurements

Date	$m5 \pm SE_{\{m5\}}$	Normalized
D20150811	0.716408 ± 0.000003	(1 ± 0.000005)
D20150827	0.715858 ± 0.000003	(1 ± 0.000004)
D20151013	0.715399 ± 0.000002	(1 ± 0.000003)
D20151222	0.716771 ± 0.000002	(1 ± 0.000003)
D20160505	0.717343 ± 0.000002	(1 ± 0.000003)
D20160628	0.715799 ± 0.000002	(1 ± 0.000003)
D20160927	0.715156 ± 0.000003	(1 ± 0.000004)

<i>D20161011</i>	<i>0.715926 ± 0.000004</i>	<i>(1 ± 0.000006)</i>
<i>D20161031</i>	<i>0.721892 ± 0.000003</i>	<i>(1 ± 0.000004)</i>
<i>D20161109</i>	<i>0.722016 ± 0.000003</i>	<i>(1 ± 0.000004)</i>
<i>D20170117</i>	<i>0.716968 ± 0.000002</i>	<i>(1 ± 0.000003)</i>

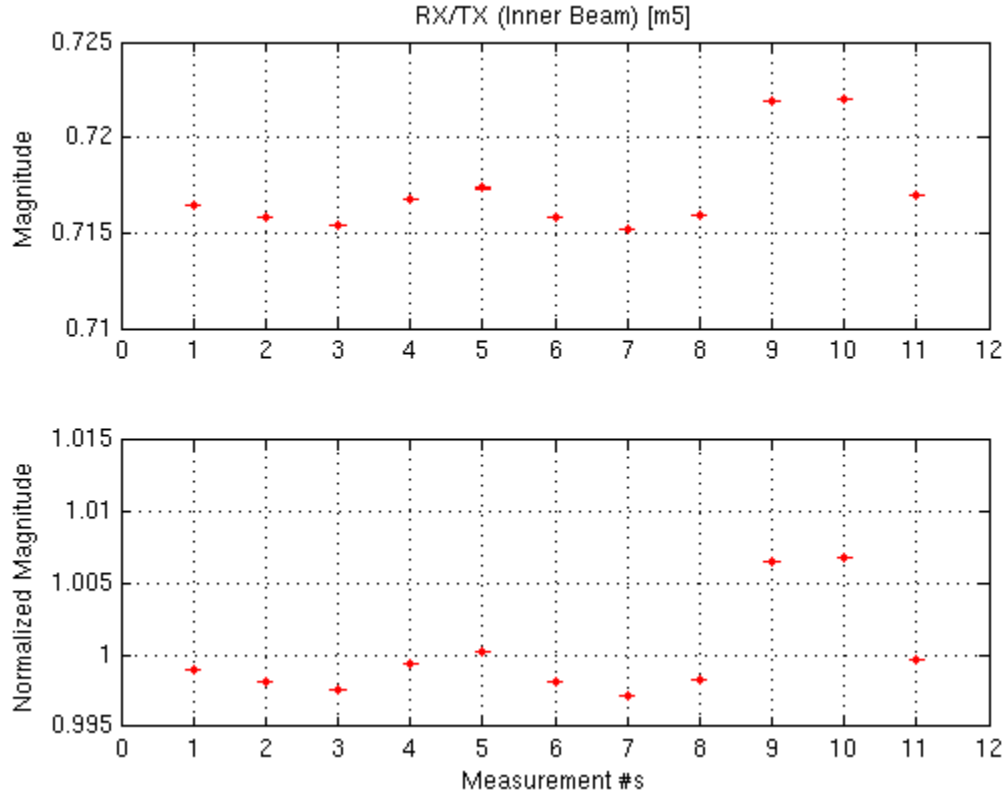

Summary of RX/TX (Inner Beam) [m5]:

<i>Mean value:</i>	<i>0.717157</i>
<i>Standard deviation:</i>	<i>0.002284</i>
<i>Standard Error:</i>	<i>0.000721</i>
<i>Relative Standard Error:</i>	<i>0.001006</i>


RX/TX Ratio (Outer Beam)

List of Measurements

<i>Date</i>	<i>m6 ± SE_{m6}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>0.726657 ± 0.000003</i>	<i>(1 ± 0.000004)</i>
<i>D20150827</i>	<i>0.726468 ± 0.000002</i>	<i>(1 ± 0.000003)</i>

LHOY-End RxPD and Tx-
PD Calibration Trends

<i>D20151013</i>	<i>0.727582 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20151222</i>	<i>0.728972 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20160505</i>	<i>0.730960 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20160628</i>	<i>0.732089 ± 0.000003</i>	<i>(1 ± 0.000004)</i>
<i>D20160927</i>	<i>0.732393 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20161011</i>	<i>0.726292 ± 0.000003</i>	<i>(1 ± 0.000004)</i>
<i>D20161031</i>	<i>0.725420 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20161109</i>	<i>0.724600 ± 0.000002</i>	<i>(1 ± 0.000003)</i>
<i>D20170117</i>	<i>0.731319 ± 0.000005</i>	<i>(1 ± 0.000007)</i>

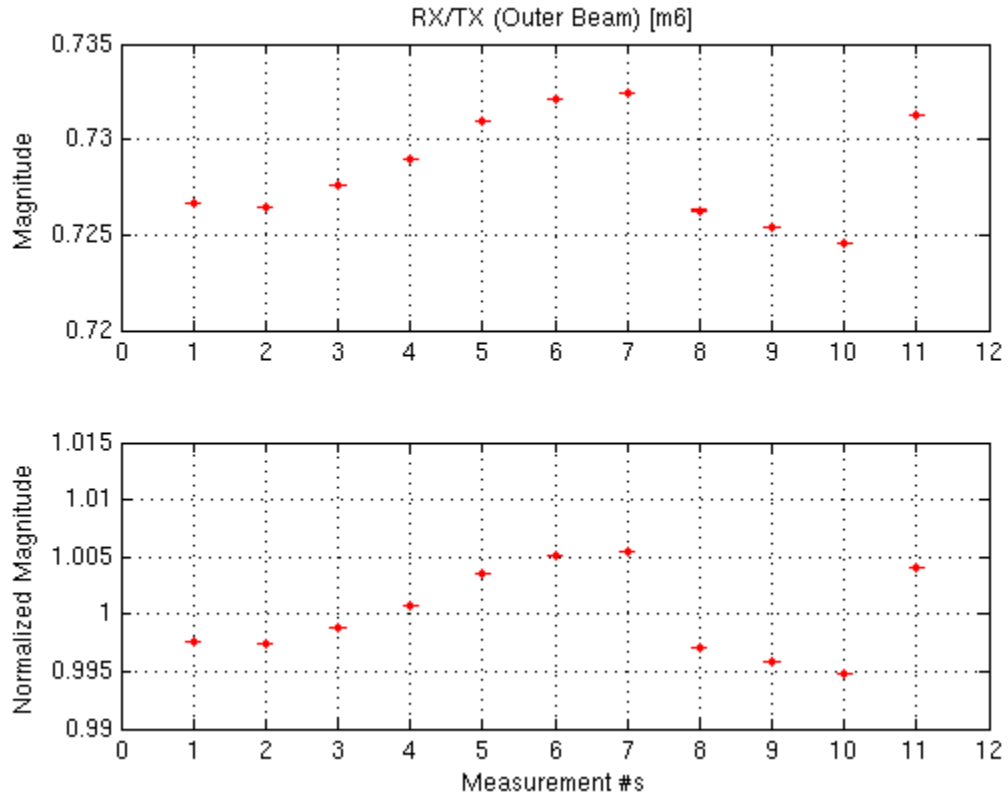


Summary of RX/TX (Outer Beam) [m6]:

<i>Mean value:</i>	<i>0.728398</i>
<i>Standard deviation:</i>	<i>0.002729</i>
<i>Standard Error:</i>	<i>0.000862</i>
<i>Relative Standard Error:</i>	<i>0.001183</i>

Optical Efficiency of Inner Beam

List of Measurements

<i>Date</i>	<i>$e_i \pm SE_{\{e_i\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>0.989808 ± 0.000062</i>	<i>(1 ± 0.000062)</i>
<i>D20150827</i>	<i>0.979224 ± 0.000052</i>	<i>(1 ± 0.000053)</i>
<i>D20151013</i>	<i>0.991448 ± 0.000049</i>	<i>(1 ± 0.000049)</i>
<i>D20151222</i>	<i>0.991154 ± 0.000057</i>	<i>(1 ± 0.000058)</i>
<i>D20160505</i>	<i>0.992086 ± 0.000061</i>	<i>(1 ± 0.000061)</i>
<i>D20160628</i>	<i>0.990643 ± 0.000059</i>	<i>(1 ± 0.000060)</i>
<i>D20160927</i>	<i>0.993815 ± 0.000065</i>	<i>(1 ± 0.000065)</i>
<i>D20161011</i>	<i>0.987658 ± 0.000074</i>	<i>(1 ± 0.000075)</i>
<i>D20161031</i>	<i>0.991589 ± 0.000060</i>	<i>(1 ± 0.000060)</i>
<i>D20161109</i>	<i>0.992628 ± 0.000157</i>	<i>(1 ± 0.000158)</i>
<i>D20170117</i>	<i>0.976747 ± 0.000185</i>	<i>(1 ± 0.000190)</i>

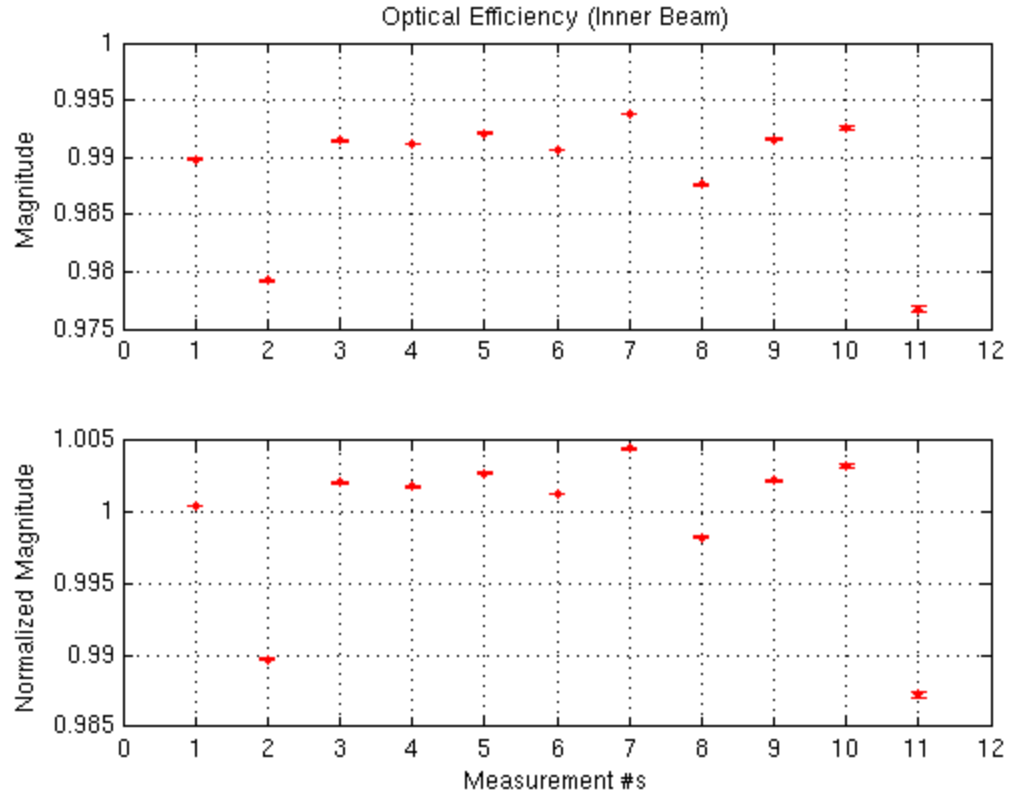

Summary of Optical Efficiency (Inner Beam):


Mean value: 0.989362
Standard deviation: 0.004759
Standard Error: 0.001503
Relative Standard Error: 0.001519

Optical Efficiency of Outer Beam

List of Measurements

Date	$e_o \pm SE_{\{e_o\}}$	Normalized
D20150811	0.986759 ± 0.000061	(1 ± 0.000062)
D20150827	0.988317 ± 0.000047	(1 ± 0.000047)
D20151013	0.987256 ± 0.000049	(1 ± 0.000050)
D20151222	0.986890 ± 0.000041	(1 ± 0.000041)
D20160505	0.986788 ± 0.000060	(1 ± 0.000061)
D20160628	0.986257 ± 0.000058	(1 ± 0.000059)
D20160927	0.989731 ± 0.000065	(1 ± 0.000066)

<i>D20161011</i>	<i>0.988909 ± 0.000070</i>	<i>(1 ± 0.000071)</i>
<i>D20161031</i>	<i>0.985153 ± 0.000061</i>	<i>(1 ± 0.000062)</i>
<i>D20161109</i>	<i>0.984771 ± 0.000150</i>	<i>(1 ± 0.000153)</i>
<i>D20170117</i>	<i>0.963290 ± 0.000993</i>	<i>(1 ± 0.001031)</i>

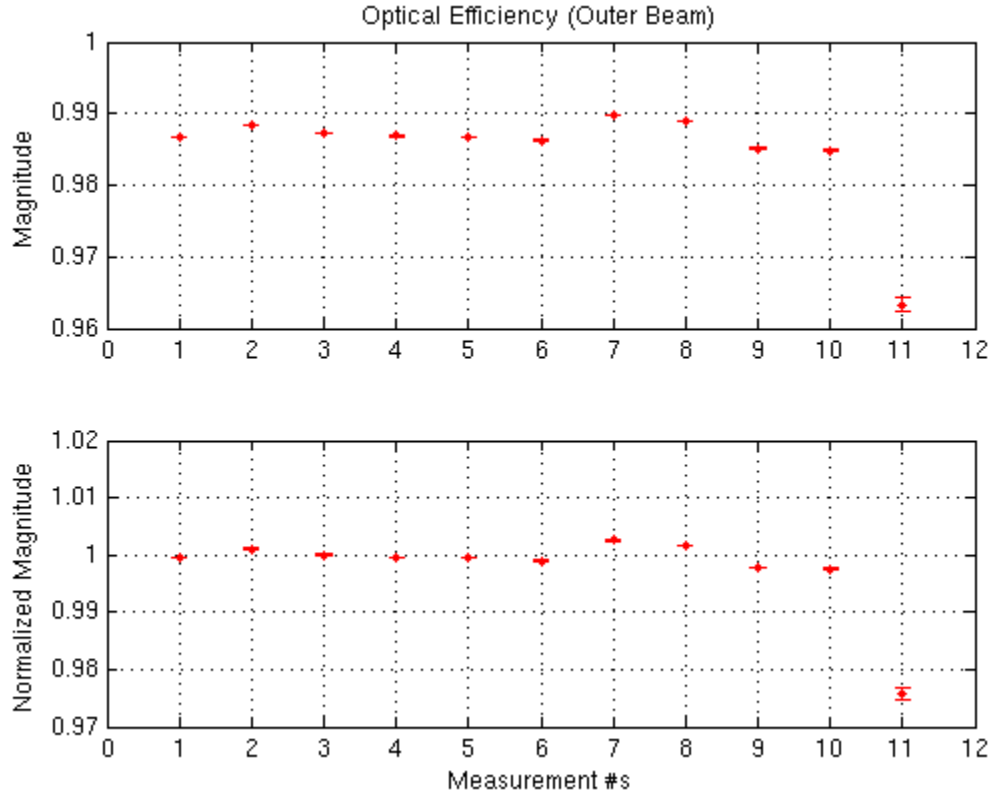

Summary of Optical Efficiency (Outer Beam):


<i>Mean value:</i>	<i>0.987230</i>
<i>Standard deviation:</i>	<i>0.001344</i>
<i>Standard Error:</i>	<i>0.000424</i>
<i>Relative Standard Error:</i>	<i>0.000430</i>

Total Optical Efficiency

List of Measurements

<i>Date</i>	<i>e ± SE_{e}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>0.988271 ± 0.000043</i>	<i>(1 ± 0.000043)</i>
<i>D20150827</i>	<i>0.983810 ± 0.000034</i>	<i>(1 ± 0.000035)</i>

D20151013	0.989331 ± 0.000034	(1 ± 0.000035)
D20151222	0.989000 ± 0.000035	(1 ± 0.000035)
D20160505	0.989405 ± 0.000042	(1 ± 0.000043)
D20160628	0.988423 ± 0.000041	(1 ± 0.000041)
D20160927	0.991746 ± 0.000046	(1 ± 0.000046)
D20161011	0.988287 ± 0.000050	(1 ± 0.000051)
D20161031	0.988353 ± 0.000042	(1 ± 0.000043)
D20161109	0.988680 ± 0.000108	(1 ± 0.000109)
D20170117	0.969941 ± 0.000492	(1 ± 0.000507)

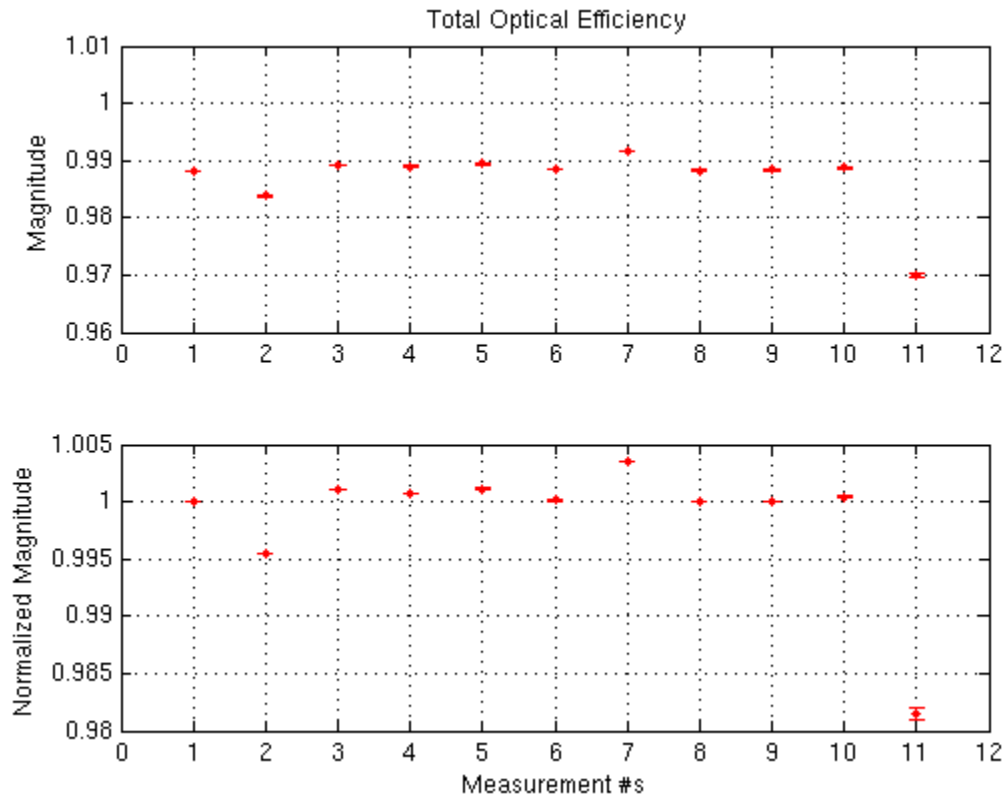


Summary of Total Optical Efficiency:

Mean value:	0.988292
Standard deviation:	0.002240
Standard Error:	0.000707
Relative Standard Error:	0.000716

TX/WS Ratio

List of Measurements

<i>Date</i>	<i>$R_{TW} \pm SE_{\{R_{TW}\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-2.742279 ± 0.000011</i>	<i>(1 ± 0.000004)</i>
<i>D20150827</i>	<i>-2.744228 ± 0.000009</i>	<i>(1 ± 0.000003)</i>
<i>D20151013</i>	<i>-2.742723 ± 0.000009</i>	<i>(1 ± 0.000003)</i>
<i>D20151222</i>	<i>-2.738239 ± 0.000009</i>	<i>(1 ± 0.000003)</i>
<i>D20160505</i>	<i>-2.763161 ± 0.000011</i>	<i>(1 ± 0.000004)</i>
<i>D20160628</i>	<i>-2.759803 ± 0.000011</i>	<i>(1 ± 0.000004)</i>
<i>D20160927</i>	<i>-2.753569 ± 0.000011</i>	<i>(1 ± 0.000004)</i>
<i>D20161011</i>	<i>-2.764191 ± 0.000014</i>	<i>(1 ± 0.000005)</i>
<i>D20161031</i>	<i>-2.744705 ± 0.000010</i>	<i>(1 ± 0.000004)</i>
<i>D20161109</i>	<i>-3.070510 ± 0.000023</i>	<i>(1 ± 0.000007)</i>
<i>D20170117</i>	<i>-3.056948 ± 0.000033</i>	<i>(1 ± 0.000011)</i>

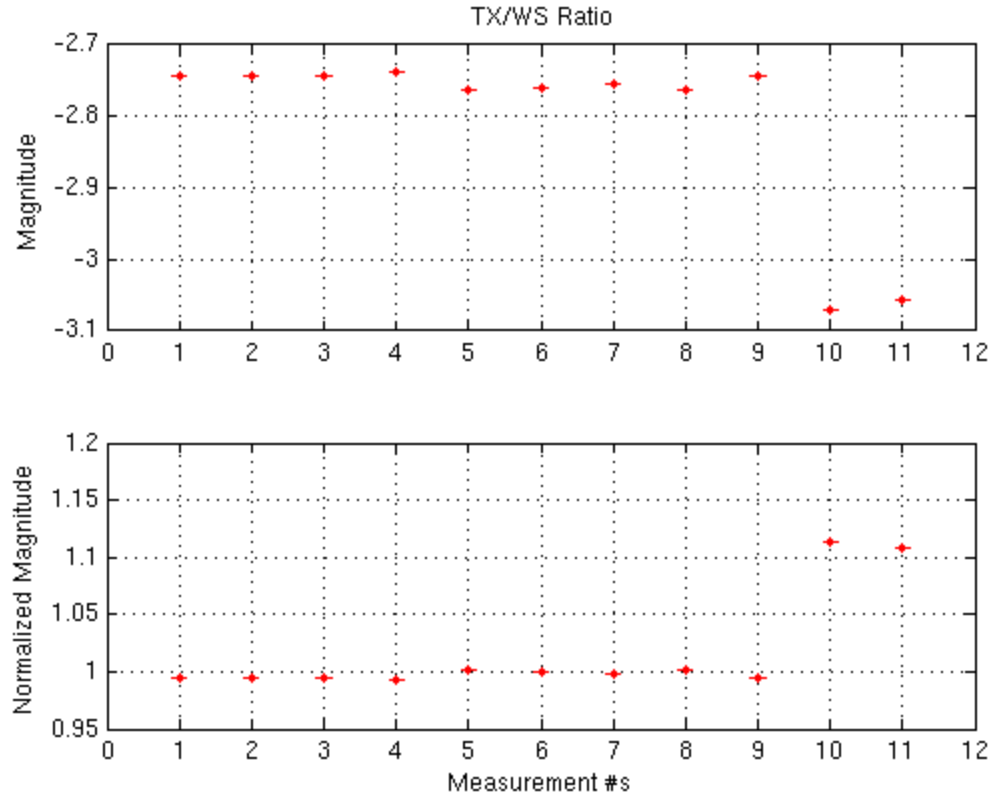

Summary of TX/WS Ratio:


Mean value: -2.759340
Standard deviation: 0.060731
Standard Error: 0.019182
Relative Standard Error: 0.006952

RX/WS Ratio

List of Measurements

Date	$R_{RW} \pm SE_{\{R_{RW}\}}$	Normalized
D20150811	-4.004239 ± 0.000126	(1 ± 0.000032)
D20150827	-4.023526 ± 0.000096	(1 ± 0.000024)
D20151013	-4.000359 ± 0.000097	(1 ± 0.000024)
D20151222	-4.002816 ± 0.000096	(1 ± 0.000024)
D20160505	-4.044736 ± 0.000119	(1 ± 0.000029)
D20160628	-4.042655 ± 0.000118	(1 ± 0.000029)
D20160927	-4.019073 ± 0.000135	(1 ± 0.000033)

<i>D20161011</i>	<i>-4.033790 ± 0.000139</i>	<i>(1 ± 0.000034)</i>
<i>D20161031</i>	<i>-4.019253 ± 0.000127</i>	<i>(1 ± 0.000032)</i>
<i>D20161109</i>	<i>-4.492703 ± 0.000378</i>	<i>(1 ± 0.000084)</i>
<i>D20170117</i>	<i>-4.564432 ± 0.002271</i>	<i>(1 ± 0.000497)</i>

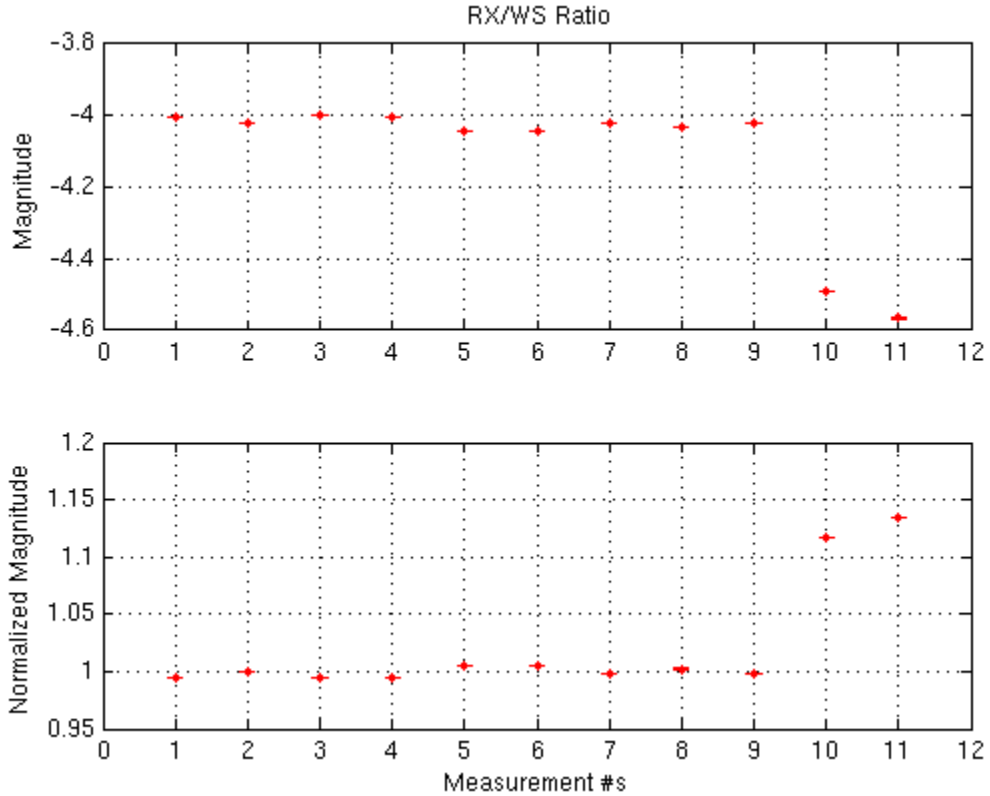

Summary of RX/WS Ratio:


<i>Mean value:</i>	<i>-4.024058</i>
<i>Standard deviation:</i>	<i>0.053010</i>
<i>Standard Error:</i>	<i>0.016743</i>
<i>Relative Standard Error:</i>	<i>0.004161</i>

TX/WS Ratio (Corrected for OE)

List of Measurements

<i>Date</i>	<i>R_Twc ± SE_{R_Twc}</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-2.758456 ± 0.000060</i>	<i>(1 ± 0.000022)</i>
<i>D20150827</i>	<i>-2.766624 ± 0.000048</i>	<i>(1 ± 0.000017)</i>

D20151013	-2.757433 ± 0.000048	(1 ± 0.000017)
D20151222	-2.753383 ± 0.000048	(1 ± 0.000018)
D20160505	-2.777877 ± 0.000059	(1 ± 0.000021)
D20160628	-2.775872 ± 0.000058	(1 ± 0.000021)
D20160927	-2.764980 ± 0.000064	(1 ± 0.000023)
D20161011	-2.780474 ± 0.000071	(1 ± 0.000025)
D20161031	-2.760782 ± 0.000059	(1 ± 0.000021)
D20161109	-3.087988 ± 0.000168	(1 ± 0.000054)
D20170117	-3.103593 ± 0.000776	(1 ± 0.000250)

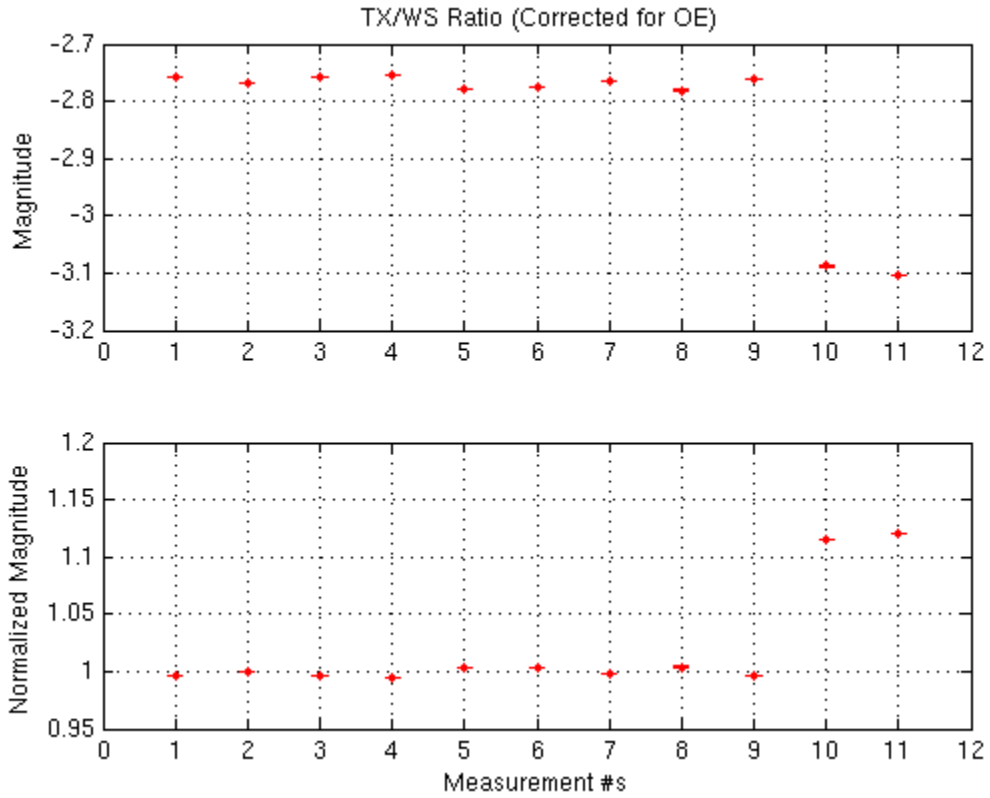


Summary of TX/WS Ratio (Corrected for OE):

Mean value:	-2.768883
Standard deviation:	0.039101
Standard Error:	0.012350
Relative Standard Error:	0.004460

RX/WS Ratio (Corrected for OE)

List of Measurements

<i>Date</i>	<i>$R_Rwc \pm SE_{\{R_Rwc\}}$</i>	<i>Normalized</i>
<i>D20150811</i>	<i>-3.980617 ± 0.000087</i>	<i>(1 ± 0.000022)</i>
<i>D20150827</i>	<i>-3.990691 ± 0.000070</i>	<i>(1 ± 0.000018)</i>
<i>D20151013</i>	<i>-3.978905 ± 0.000069</i>	<i>(1 ± 0.000017)</i>
<i>D20151222</i>	<i>-3.980678 ± 0.000070</i>	<i>(1 ± 0.000018)</i>
<i>D20160505</i>	<i>-4.023196 ± 0.000086</i>	<i>(1 ± 0.000021)</i>
<i>D20160628</i>	<i>-4.019117 ± 0.000084</i>	<i>(1 ± 0.000021)</i>
<i>D20160927</i>	<i>-4.002417 ± 0.000092</i>	<i>(1 ± 0.000023)</i>
<i>D20161011</i>	<i>-4.010027 ± 0.000103</i>	<i>(1 ± 0.000026)</i>
<i>D20161031</i>	<i>-3.995710 ± 0.000086</i>	<i>(1 ± 0.000022)</i>
<i>D20161109</i>	<i>-4.467129 ± 0.000243</i>	<i>(1 ± 0.000054)</i>
<i>D20170117</i>	<i>-4.494785 ± 0.001126</i>	<i>(1 ± 0.000251)</i>

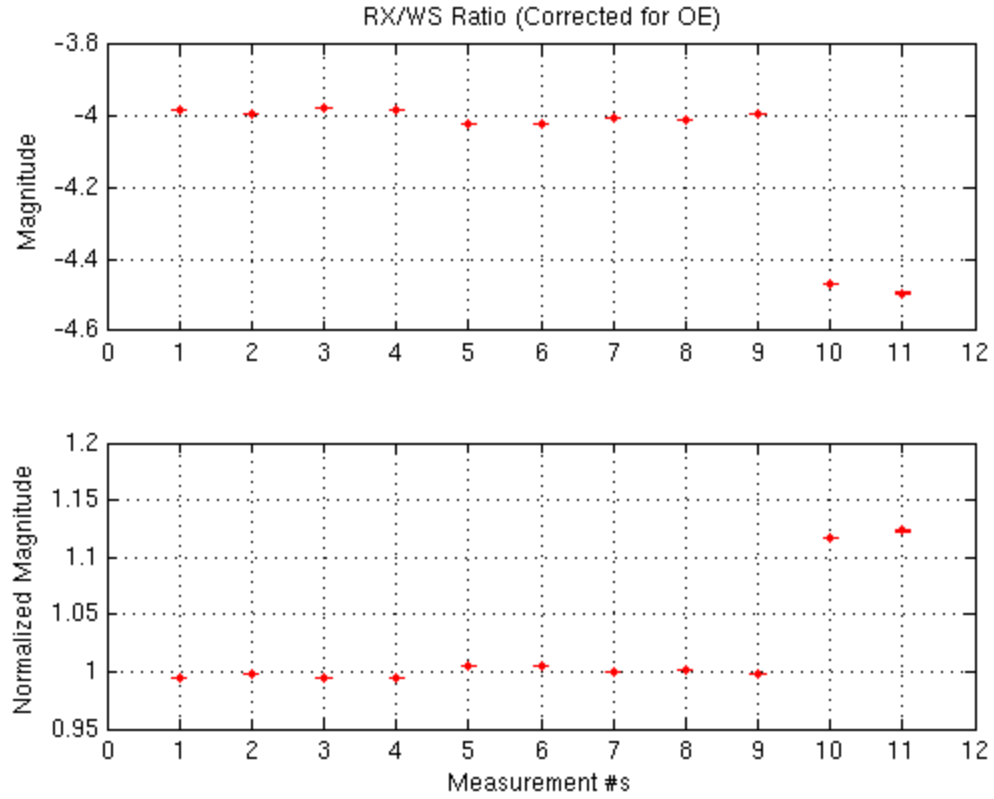

Summary of RX/WS Ratio (Corrected for OE):


Mean value: -4.001481
Standard deviation: 0.058160
Standard Error: 0.018370
Relative Standard Error: 0.004591

Power Imbalance

List of Measurements

D20150811	0.983938 ± 0.000059	(1 ± 0.000059)
D20150827	0.982844 ± 0.000050	(1 ± 0.000051)
D20151013	0.980135 ± 0.000048	(1 ± 0.000049)
D20151222	0.979459 ± 0.000051	(1 ± 0.000052)
D20160505	0.976585 ± 0.000060	(1 ± 0.000062)
D20160628	0.974999 ± 0.000057	(1 ± 0.000059)
D20160927	0.973728 ± 0.000061	(1 ± 0.000063)
D20161011	0.989087 ± 0.000075	(1 ± 0.000075)

<i>D20161031</i>	<i>0.989175 ± 0.000057</i>	<i>(1 ± 0.000058)</i>
<i>D20161109</i>	<i>0.990030 ± 0.000137</i>	<i>(1 ± 0.000138)</i>
<i>D20170117</i>	<i>0.977093 ± 0.000199</i>	<i>(1 ± 0.000204)</i>

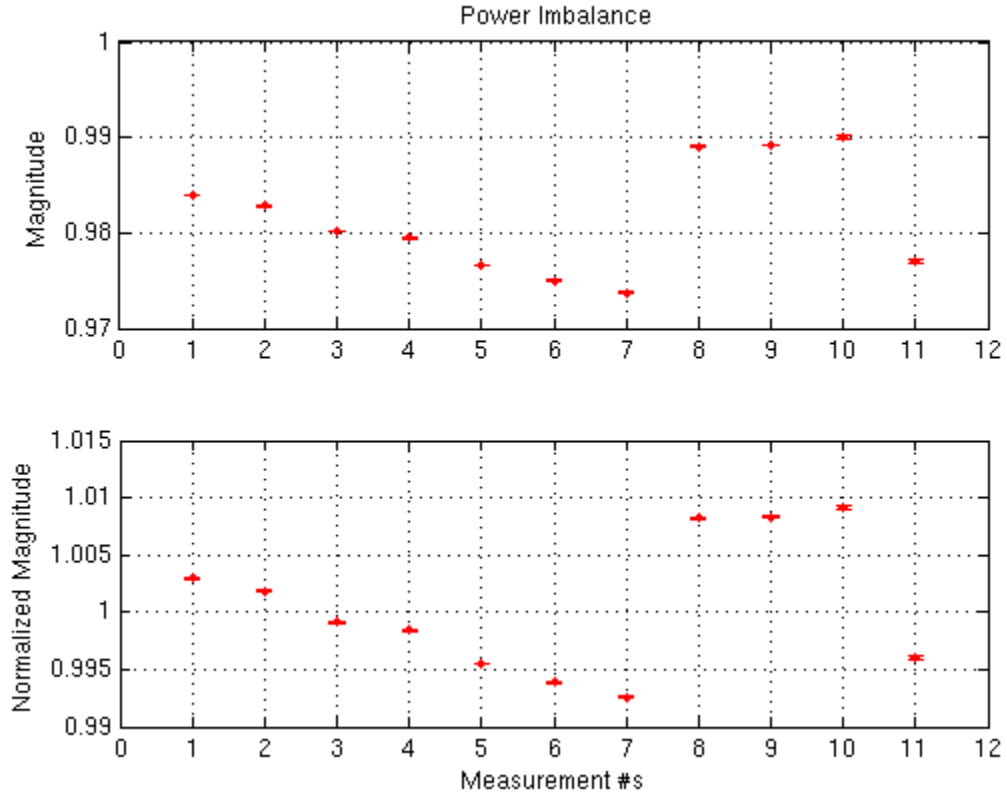

Summary of Power Imbalance:

<i>Mean value:</i>	<i>0.981011</i>
<i>Standard deviation:</i>	<i>0.005226</i>
<i>Standard Error:</i>	<i>0.001651</i>
<i>Relative Standard Error:</i>	<i>0.001683</i>

Summary

<i>Description</i>	<i>Value</i>	<i>Std Dev</i>	<i>Std Err</i>	<i>Rel Err:</i>
<i>OE (e)</i>	<i>0.9883</i>	<i>0.0022</i>	<i>0.0007</i>	<i>0.0007</i>
<i>TX/WS (a1a2)</i>	<i>-2.7689</i>	<i>0.0391</i>	<i>0.0124</i>	<i>0.0045</i>
<i>RX/WS (b1b2)</i>	<i>-4.0015</i>	<i>0.0582</i>	<i>0.0184</i>	<i>0.0046</i>
<i>w (a5)</i>	<i>1.0000</i>	<i>----</i>	<i>----</i>	<i>0.0034</i>