

RxPD and TxPD Calibration Trends

| GENERATED FOR LHO_EndX

Report Generated on August 22, 2023

Contents

1	About	1
2	WS/Tx Ratio when WS is at Tx (Inner Beam)	2
3	WS/Tx Ratio when WS is at Tx (Outer Beam)	3
4	Tx/WS responsivity ratio $\alpha_{TW} = 1/[\mathbf{m1} + \mathbf{m2}]$	4
5	WS/Tx Ratio when WS is at Rx (Inner Beam)	5
6	WS/Tx Ratio when WS is at Rx (Outer Beam)	6
7	RX/TX Ratio (Inner Beam)	7
8	Rx/Tx Ratio (Outer Beam)	8
9	m5/m3 Ratio	9
10	m6/m4 Ratio	10
11	Rx/WS responsivity ratio $\alpha_{RW} = \frac{1}{2} [\mathbf{m5}/\mathbf{m3} + \mathbf{m6}/\mathbf{m4}]$	11
12	ADC conversion factor (ζ)	12
13	TxPD calibration ($\rho_{Tx} = \rho_G \cdot \alpha_{WG} \cdot \alpha_{TW} \cdot \zeta$)	13
14	RxPD calibration ($\rho_{Rx} = \rho_G \cdot \alpha_{WG} \cdot \alpha_{RW} \cdot \zeta$)	14
15	Optical Efficiency of Inner Beam $e^i = \mathbf{m3}/\mathbf{m1}$	15
16	Optical Efficiency of Outer Beam $e^o = \mathbf{m4}/\mathbf{m2}$	16
17	Total Optical Efficiency $e = (\mathbf{m3} + \mathbf{m4})/(\mathbf{m1} + \mathbf{m2})$	17
18	Input/Output optical efficiency ratio (β)	18
19	Input Optical efficiency correction factor ($\eta_T = \sqrt{e/\beta}$)	19
20	Output Optical efficiency correction factor ($\eta_R = \sqrt{e/\beta}$)	20

21 TxPD calibration at ETM ($\rho'_{Tx} = \rho_T \cdot \eta_T \cdot \zeta$)	21
22 RxPD calibration at ETM ($\rho'_{Rx} = \rho_R \cdot \eta_R \cdot \zeta$)	22
23 Power Imbalance	23

1 About

This document contains the Pcal Calibration trends. It includes the ratios measured at the end-station labeled as m1, m2m6 as well as the quantities derived from these six ratio measurements, namely α_{TW} , α_{RW} , optical efficiency and power imbalance. This document also includes the trend of the ADC conversion factor. The sections 17 to 20 shows the trend of the parameters calculated from the derived quantities, which include Input/Output optical efficiency correction factors and Tx/Rx PD calibration factors.

Understanding Each Section


Each section contains a list of measurements with the mean value (m1), standard deviation on the mean (SD_m1) and a ratio of the standard deviation of the quantity and error bars for each measurement (frac). The list is followed by two plot figures with Magnitude on the Y axis and Index on the X axis for the first plot and the Magnitude on the Y axis and time on the X axis for the second. The error bars of each data point is the standard deviation SD_m1. Each section ends with a summary that contains the mean (the red line on the plot) along with their Standard Deviation, Std Err and Rel Err (the pink band on the plot) where each of these terms are defined as:

```
Mean = sum(x(i))/n
Std_Dev = sqrt(sum((x(i)-x_mean)^2)/(n-1))
Std_Err = Std_Dev*Student's_t_correction/sqrt(n)
Rel_Err = Std_Err/Mean
```

2 WS/Tx Ratio when WS is at Tx (Inner Beam)

List of Measurements

Date	m1 $\pm$ SD_m1
D20230110	-0.4584 $\pm$ 0.0004
D20230207	-0.4582 $\pm$ 0.0003
D20230228	-0.4576 $\pm$ 0.0003
D20230314	-0.4582 $\pm$ 0.0003
D20230404	-0.4585 $\pm$ 0.0004
D20230613	-0.4610 $\pm$ 0.0003
D20230821	-0.4607 $\pm$ 0.0003

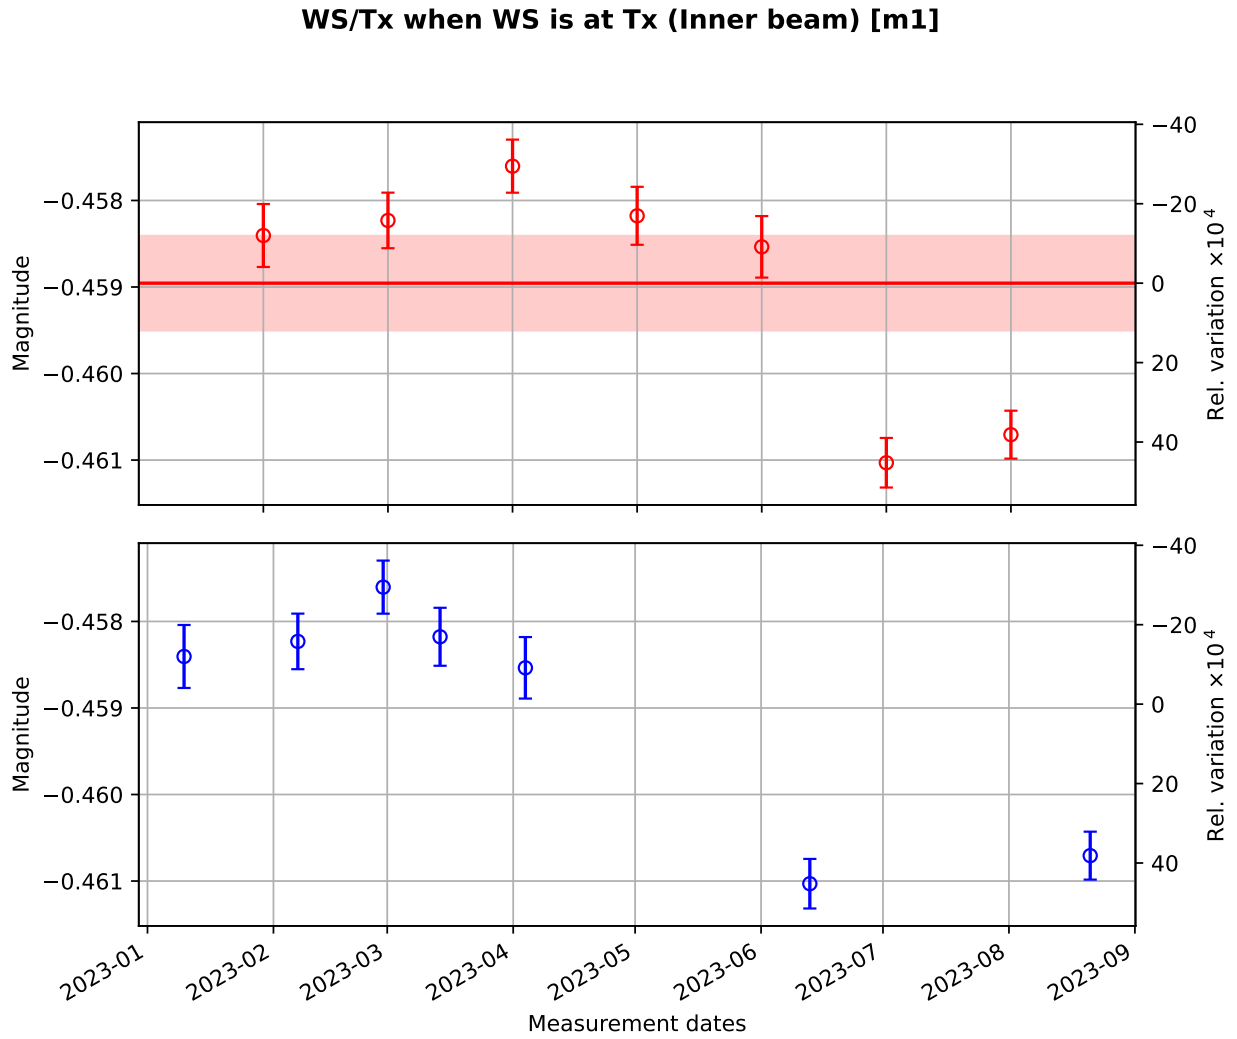


Summary of WS/Tx when WS is at Tx (Inner beam) [m1]	
Mean value:	-0.458956
Standard deviation:	0.001342
Standard error:	0.000546
Relative Standard error:	-0.001190

3 WS/Tx Ratio when WS is at Tx (Outer Beam)

List of Measurements

Date	m2 $\pm$ SD_m2
D20230110	-0.4654 $\pm$ 0.0003
D20230207	-0.4660 $\pm$ 0.0003
D20230228	-0.4663 $\pm$ 0.0003
D20230314	-0.4659 $\pm$ 0.0003
D20230404	-0.4658 $\pm$ 0.0003
D20230613	-0.4640 $\pm$ 0.0003
D20230821	-0.4643 $\pm$ 0.0003

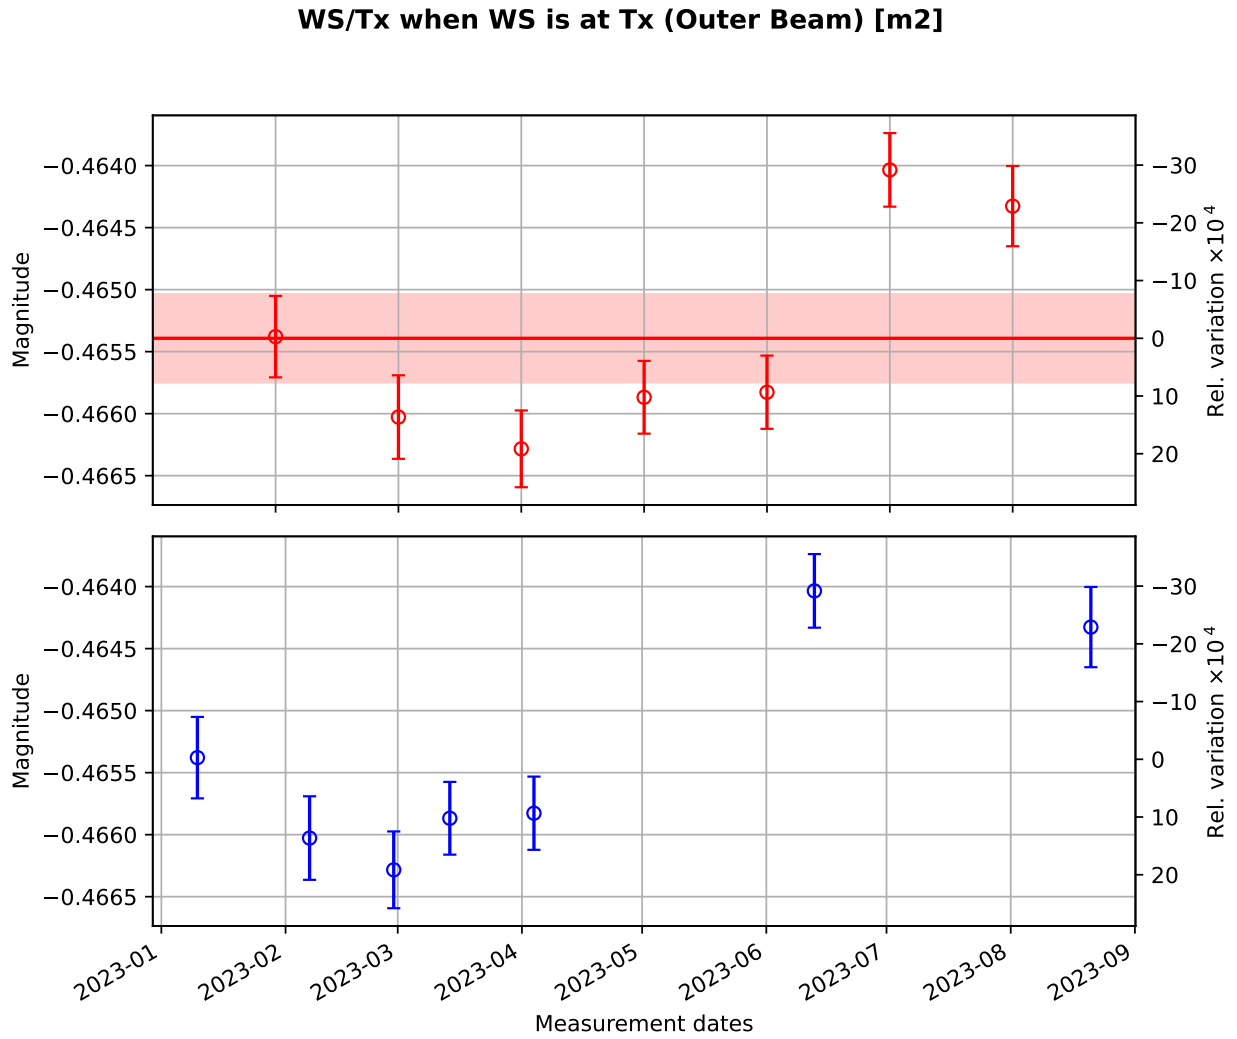


Summary of WS/Tx when WS is at Tx (Outer Beam) [m2]	
Mean value:	-0.465392
Standard deviation:	0.000875
Standard error:	0.000356
Relative Standard error:	-0.000765

4 Tx/WS responsivity ratio $\alpha_{TW} = 1/[m1 + m2]$

List of Measurements

Date	TXWS $\pm$ SD_TXWS
D20230110	-1.0825 $\pm$ 0.0005
D20230207	-1.0819 $\pm$ 0.0005
D20230228	-1.0824 $\pm$ 0.0004
D20230314	-1.0822 $\pm$ 0.0004
D20230404	-1.0818 $\pm$ 0.0005
D20230613	-1.0810 $\pm$ 0.0004
D20230821	-1.0810 $\pm$ 0.0004

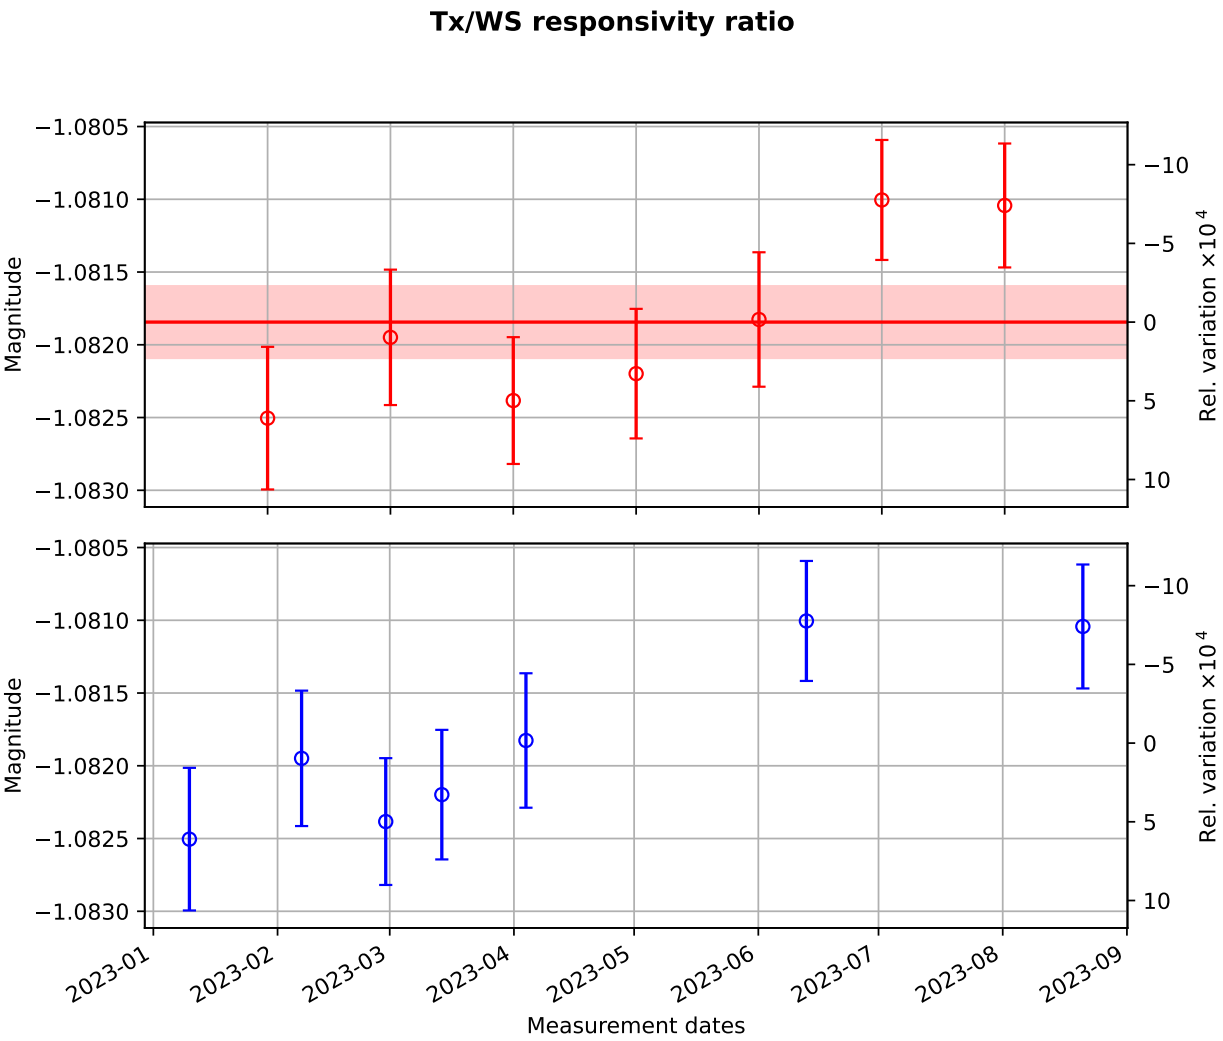


Summary of Tx/WS responsivity ratio		
Mean value:	-1.081844	
Standard deviation:	0.000607	
Standard error:	0.000247	
Relative Standard error:	-0.000228	

5 WS/Tx Ratio when WS is at Rx (Inner Beam)

List of Measurements

Date	m3 $\pm$ SD_m3
D20230110	-0.4529 $\pm$ 0.0003
D20230207	-0.4522 $\pm$ 0.0003
D20230228	-0.4518 $\pm$ 0.0003
D20230314	-0.4518 $\pm$ 0.0003
D20230404	-0.4525 $\pm$ 0.0003
D20230613	-0.4549 $\pm$ 0.0003
D20230821	-0.4541 $\pm$ 0.0003

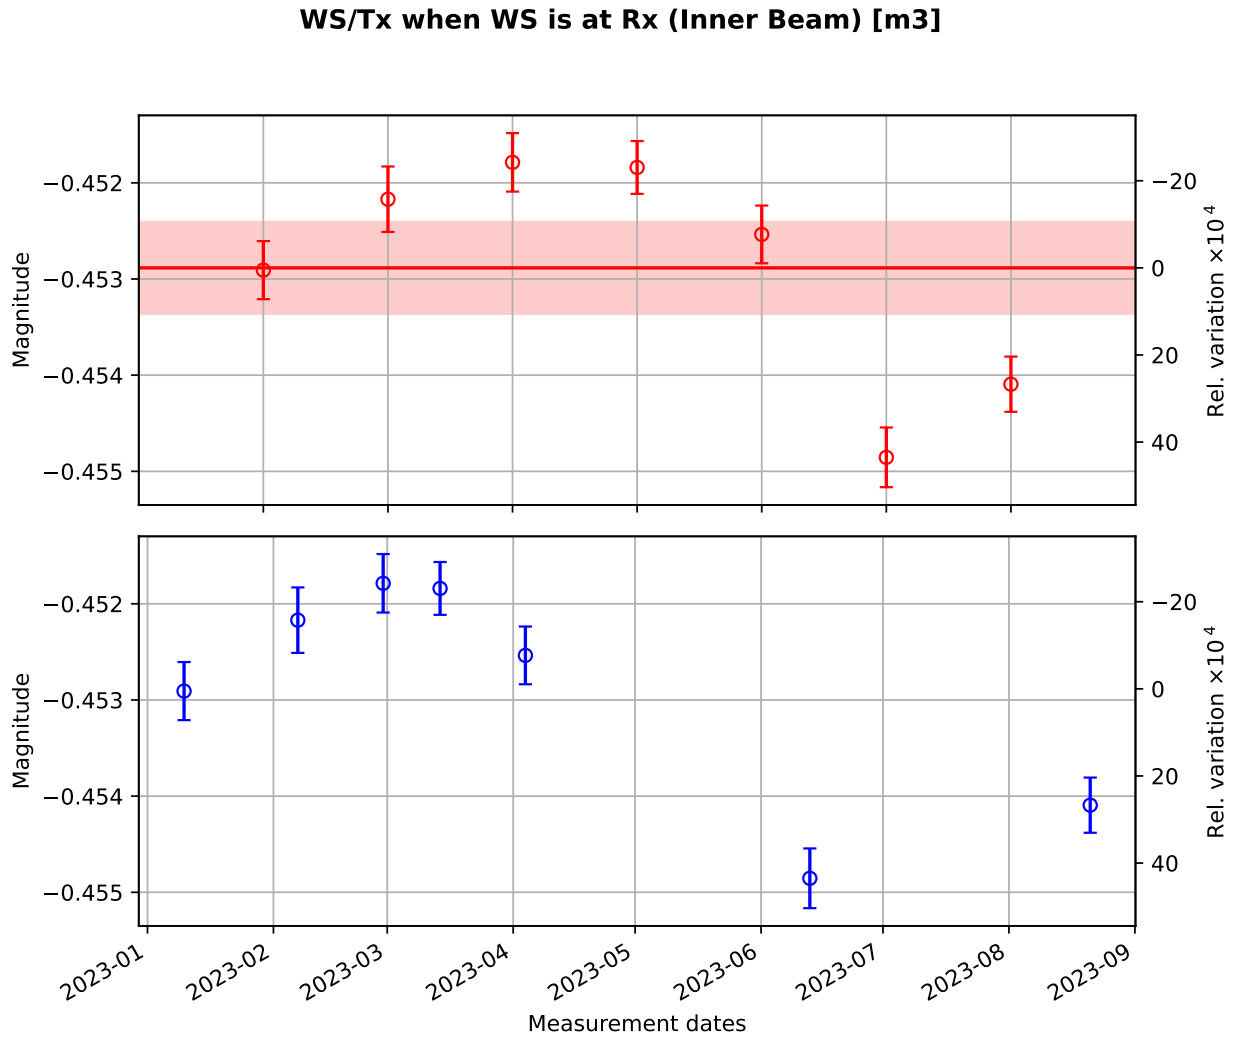


Summary of WS/Tx when WS is at Rx (Inner Beam) [m3]		
Mean value:	-0.452884	
Standard deviation:	0.001174	
Standard error:	0.000478	
Relative Standard error:	-0.001055	

6 WS/Tx Ratio when WS is at Rx (Outer Beam)

List of Measurements

Date	m4 $\pm$ SD_m4
D20230110	-0.4596 $\pm$ 0.0003
D20230207	-0.4603 $\pm$ 0.0003
D20230228	-0.4614 $\pm$ 0.0003
D20230314	-0.4606 $\pm$ 0.0003
D20230404	-0.4609 $\pm$ 0.0003
D20230613	-0.4571 $\pm$ 0.0003
D20230821	-0.4579 $\pm$ 0.0003

WS/Tx when WS is at Rx (Outer Beam) [m4]

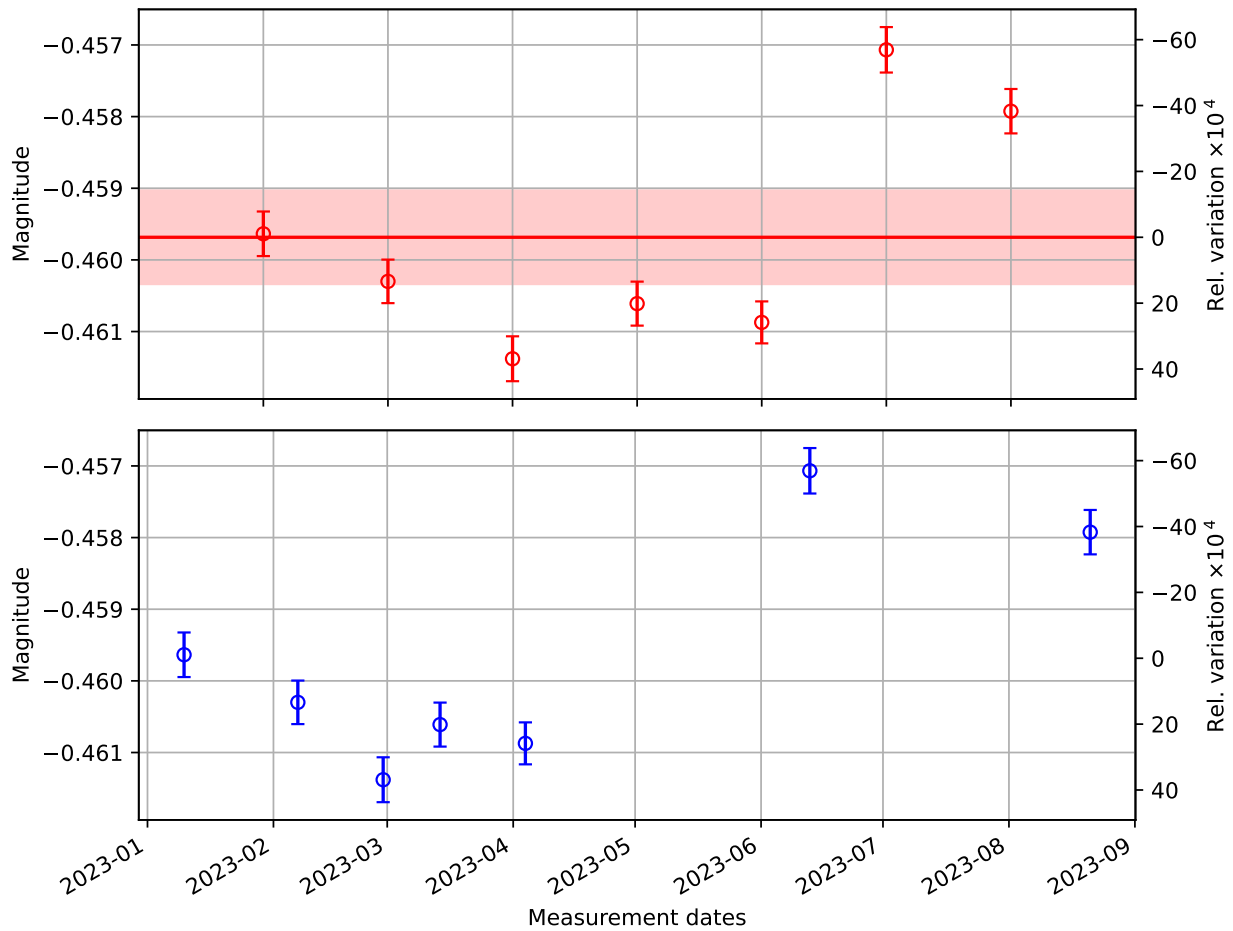


Summary of WS/Tx when WS is at Rx (Outer Beam) [m4]

Mean value:	-0.459684
Standard deviation:	0.001606
Standard error:	0.000653
Relative Standard error:	-0.001421

7 RX/TX Ratio (Inner Beam)

List of Measurements

Date	m5 $\pm$ SD_m5
D20230110	0.6295 $\pm$ 0.0002
D20230207	0.6290 $\pm$ 0.0003
D20230228	0.6280 $\pm$ 0.0002
D20230314	0.6279 $\pm$ 0.0002
D20230404	0.6288 $\pm$ 0.0002
D20230613	0.6312 $\pm$ 0.0002
D20230821	0.6296 $\pm$ 0.0002

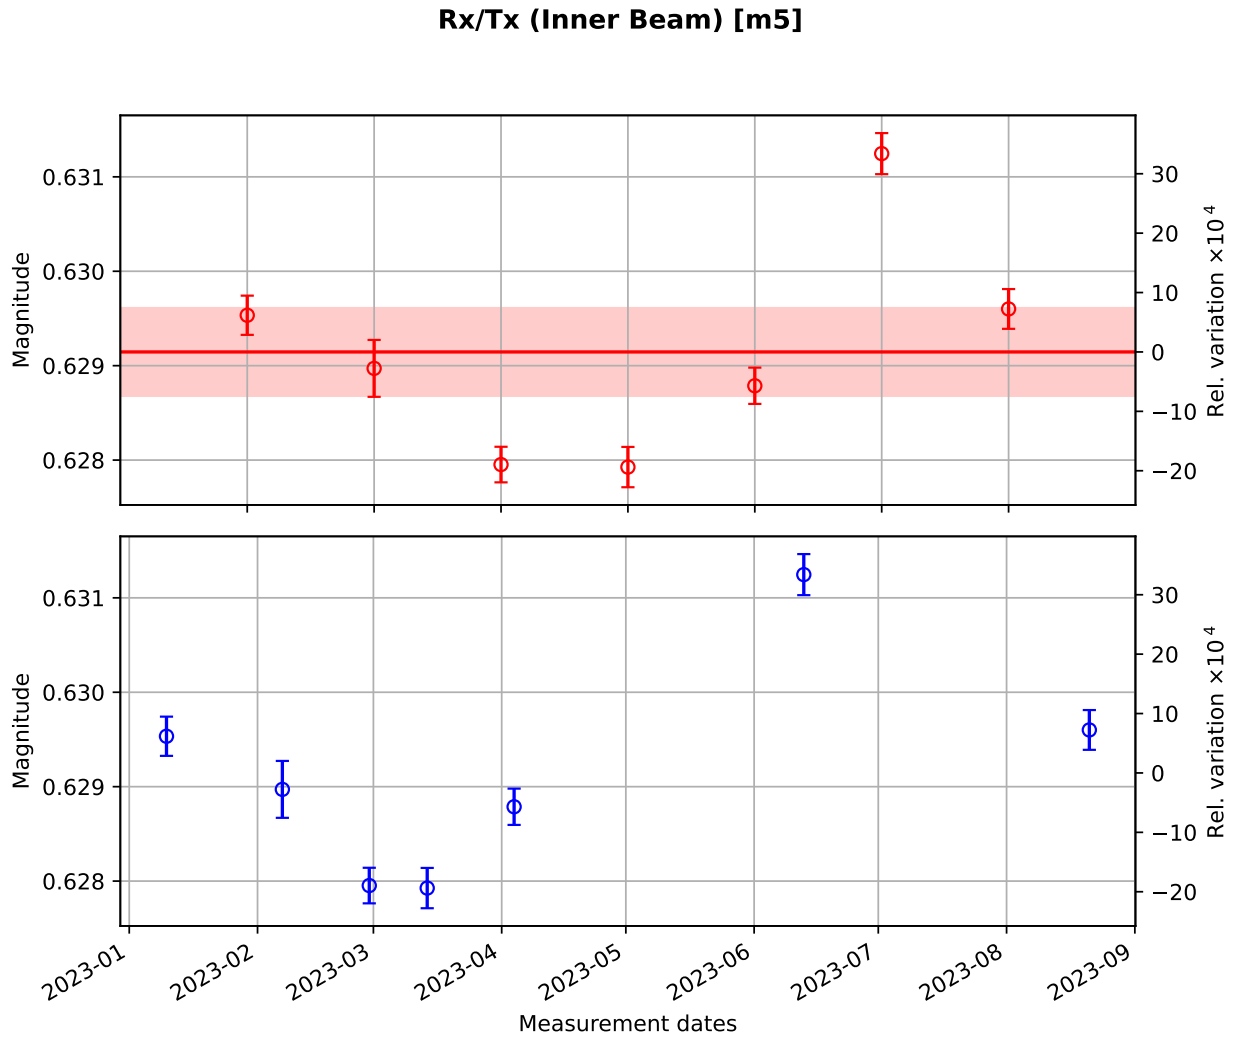


Summary of Rx/Tx (Inner Beam) [m5]		
Mean value:	0.629145	
Standard deviation:	0.001143	
Standard error:	0.000465	
Relative Standard error:	0.000739	

8 Rx/Tx Ratio (Outer Beam)

List of Measurements

Date	m6 ± SD_m6
D20230110	0.6372 ± 0.0002
D20230207	0.6369 ± 0.0002
D20230228	0.6401 ± 0.0002
D20230314	0.6394 ± 0.0002
D20230404	0.6392 ± 0.0002
D20230613	0.6332 ± 0.0002
D20230821	0.6347 ± 0.0002

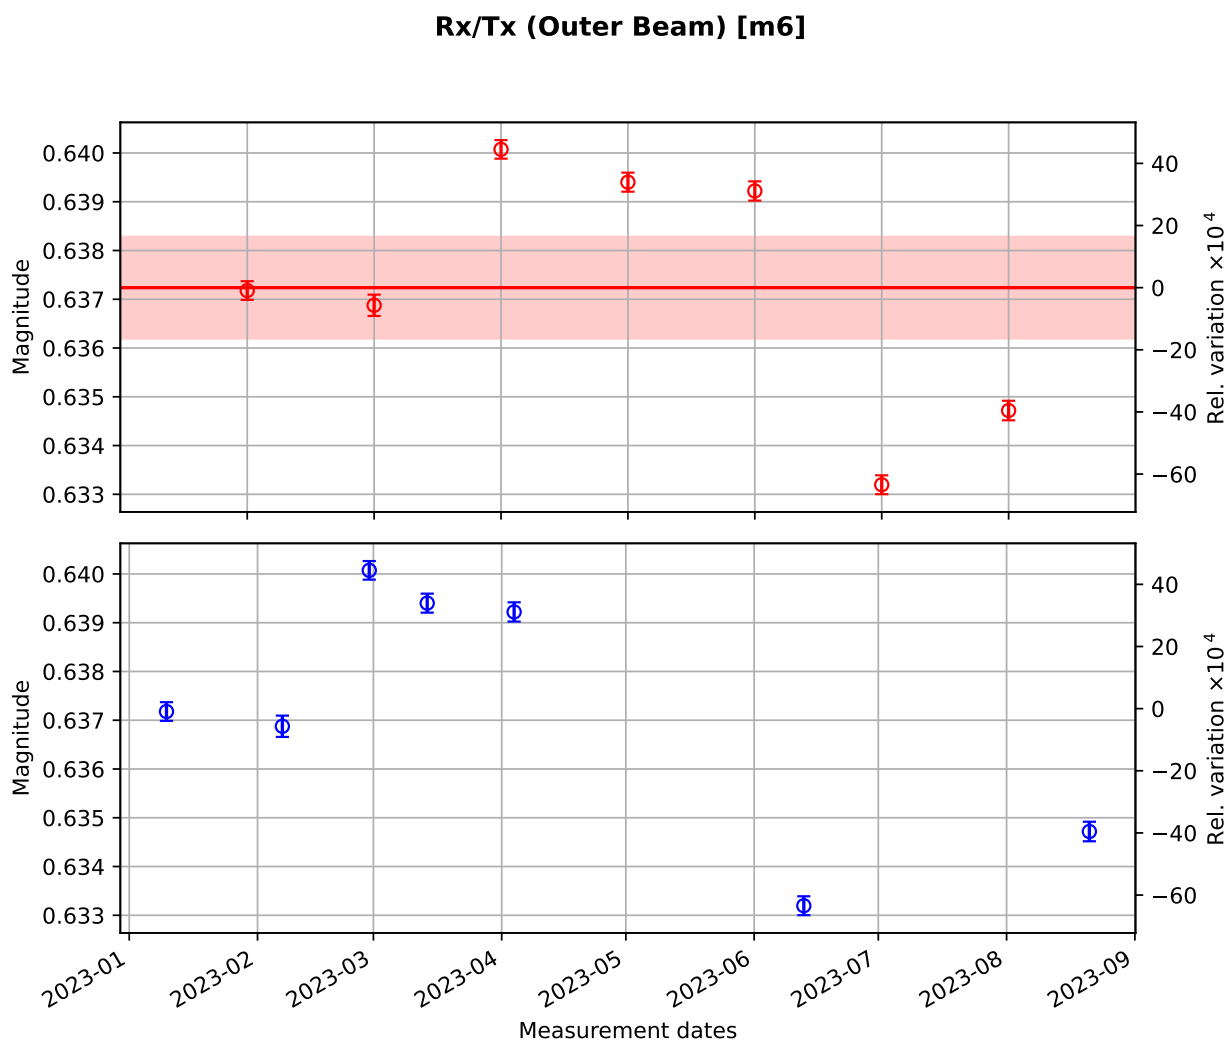


Summary of Rx/Tx (Outer Beam) [m6]		
Mean value:	0.637238	
Standard deviation:	0.002565	
Standard error:	0.001044	
Relative Standard error:	0.001638	

9 m5/m3 Ratio

List of Measurements

Date	RiTWrIT ± SD_RiTWrIT
D20230110	-1.3900 ± 0.0004
D20230207	-1.3910 ± 0.0005
D20230228	-1.3899 ± 0.0004
D20230314	-1.3897 ± 0.0003
D20230404	-1.3895 ± 0.0004
D20230613	-1.3878 ± 0.0004
D20230821	-1.3865 ± 0.0004

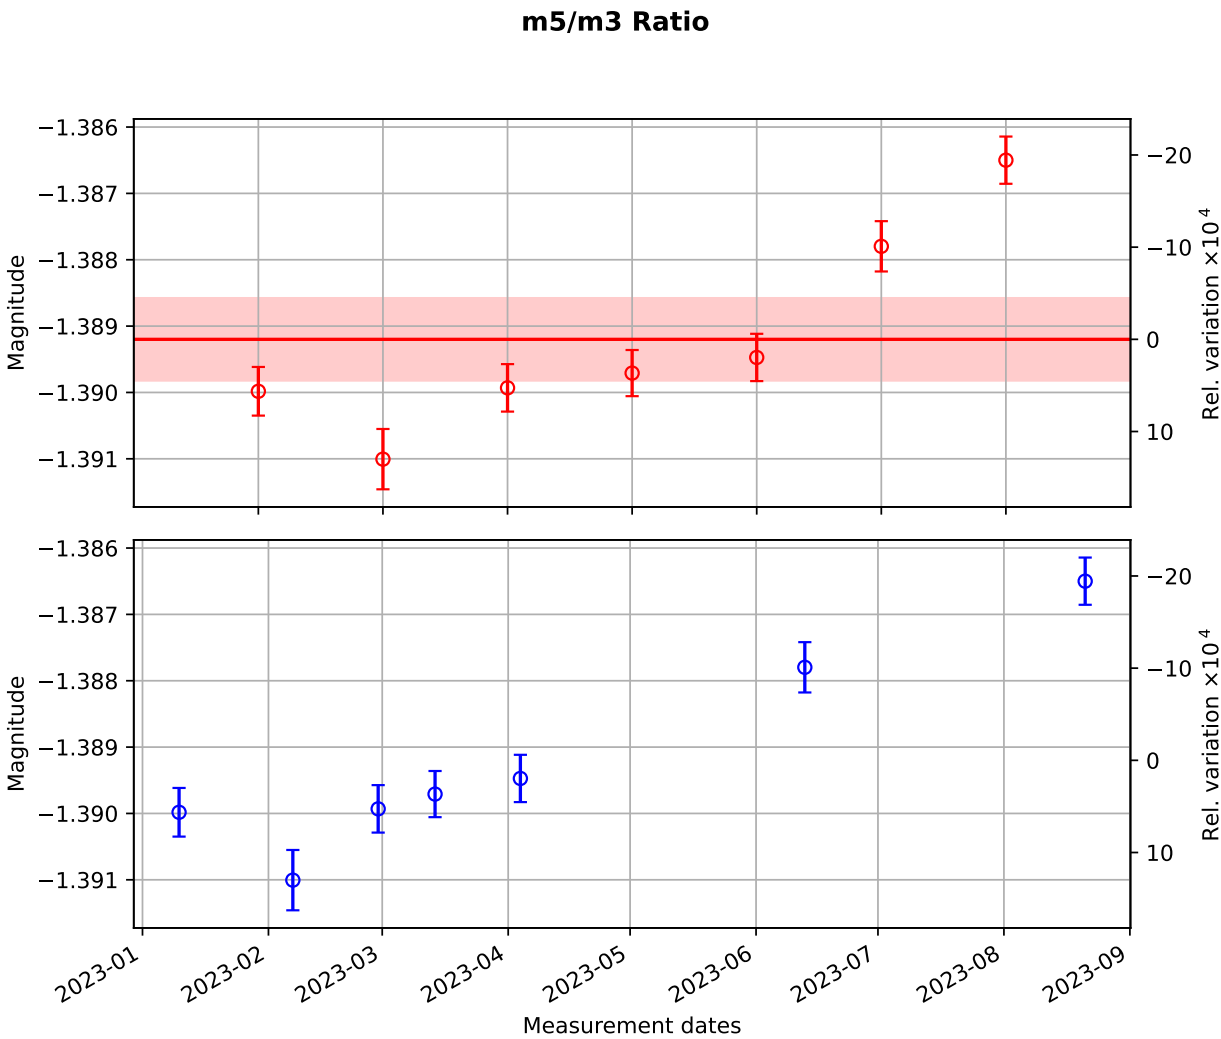


Summary of m5/m3 Ratio		
Mean value:	-1.389199	
Standard deviation:	0.001527	
Standard error:	0.000622	
Relative Standard error:	-0.000447	

10 m6/m4 Ratio

List of Measurements

Date	RoTWroT $\pm$ SD_RoTWroT
D20230110	-1.3863 $\pm$ 0.0004
D20230207	-1.3836 $\pm$ 0.0004
D20230228	-1.3873 $\pm$ 0.0004
D20230314	-1.3882 $\pm$ 0.0004
D20230404	-1.3870 $\pm$ 0.0004
D20230613	-1.3853 $\pm$ 0.0004
D20230821	-1.3861 $\pm$ 0.0004

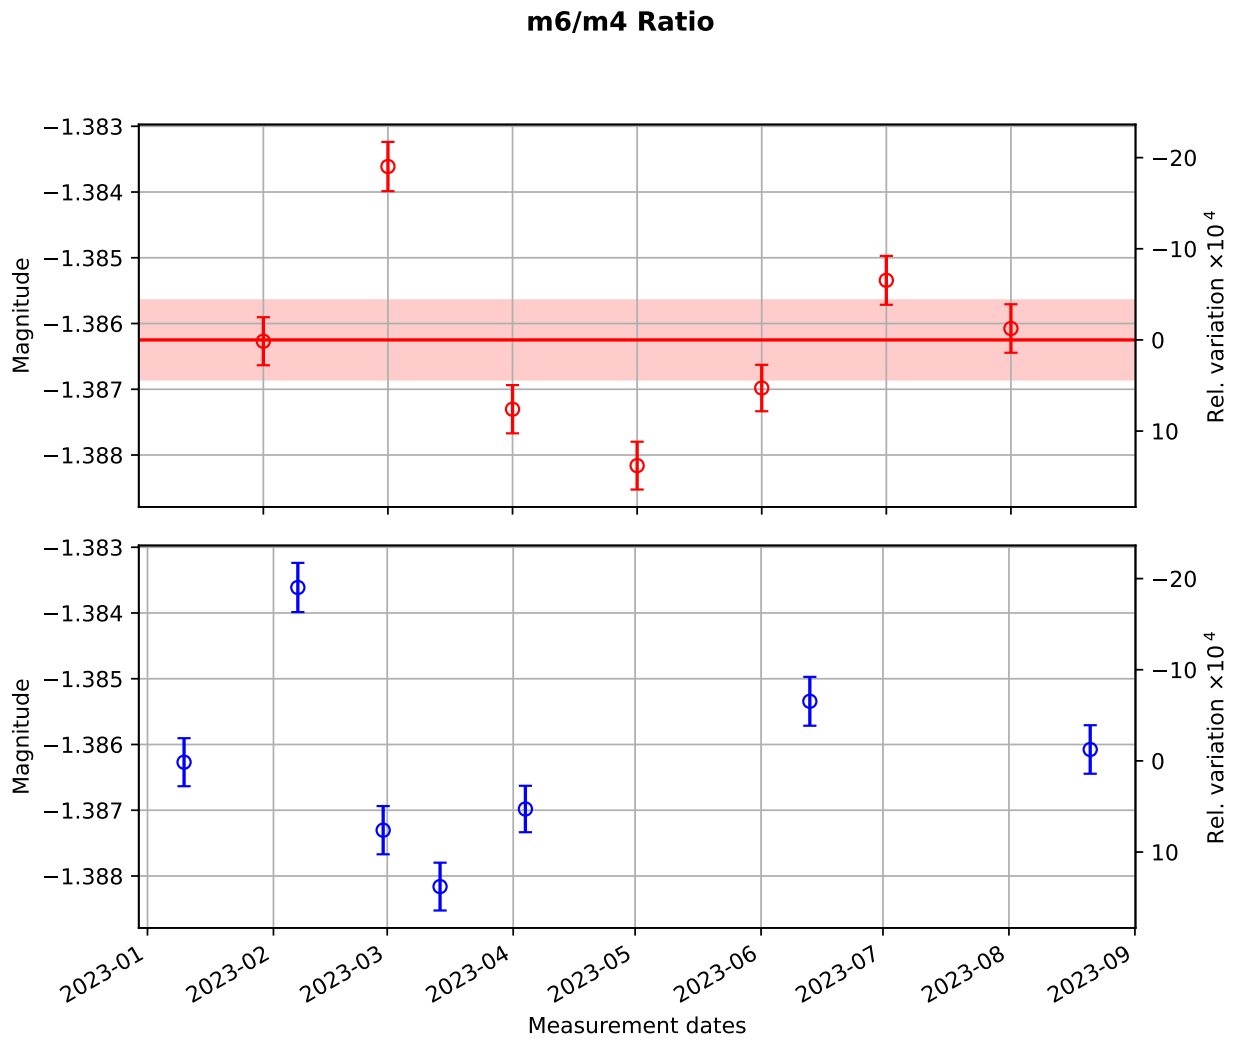


Summary of m6/m4 Ratio

Mean value:	-1.386250
Standard deviation:	0.001478
Standard error:	0.000602
Relative Standard error:	-0.000434

11 Rx/WS responsivity ratio $\alpha_{RW} = \frac{1}{2} [\mathbf{m5/m3} + \mathbf{m6/m4}]$

List of Measurements

Date	RXWS $\pm$ SD_RXWS
D20230110	-1.3881 $\pm$ 0.0004
D20230207	-1.3873 $\pm$ 0.0004
D20230228	-1.3886 $\pm$ 0.0004
D20230314	-1.3889 $\pm$ 0.0003
D20230404	-1.3882 $\pm$ 0.0003
D20230613	-1.3866 $\pm$ 0.0004
D20230821	-1.3863 $\pm$ 0.0004

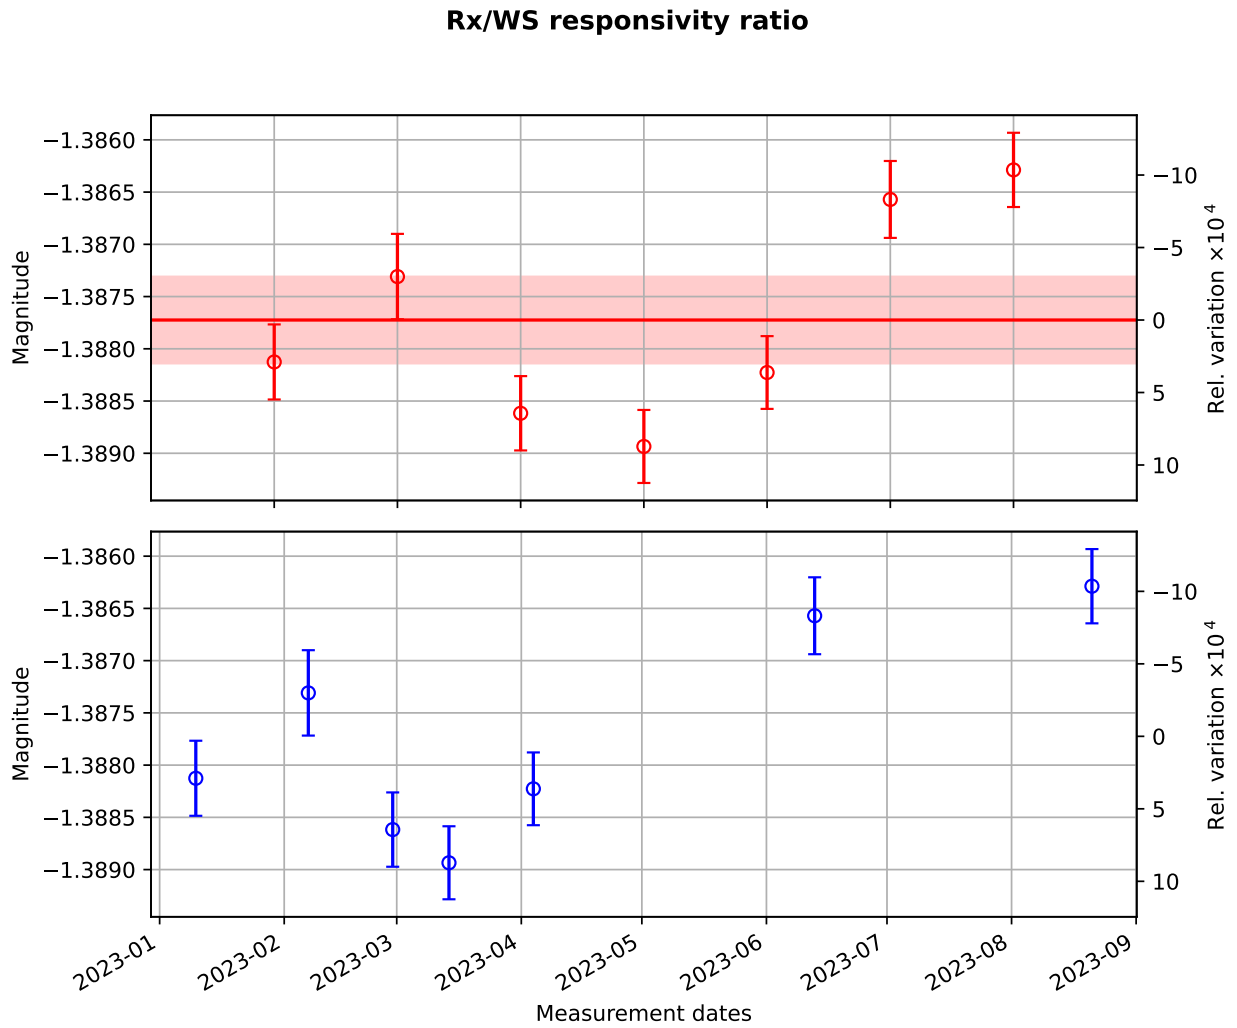

Summary of Rx/WS responsivity ratio


Mean value:	-1.387724
Standard deviation:	0.001020
Standard error:	0.000415
Relative Standard error:	-0.000299

12 ADC conversion factor (ζ)

List of Measurements

Date	$\zeta \pm \text{SD}_\zeta$
D20230110	$1.6367\text{e}+03 \pm 1.0000\text{e}-09$
D20230207	$1.6368\text{e}+03 \pm 1.0000\text{e}-09$
D20230228	$1.6367\text{e}+03 \pm 1.0000\text{e}-09$
D20230314	$1.6369\text{e}+03 \pm 1.0000\text{e}-09$
D20230404	$1.6369\text{e}+03 \pm 1.0000\text{e}-09$
D20230613	$1.6369\text{e}+03 \pm 1.0000\text{e}-09$
D20230821	$1.6368\text{e}+03 \pm 1.0000\text{e}-09$

ADC conversion factor discrepancy ($1638.4 - \zeta$ (ct/V))

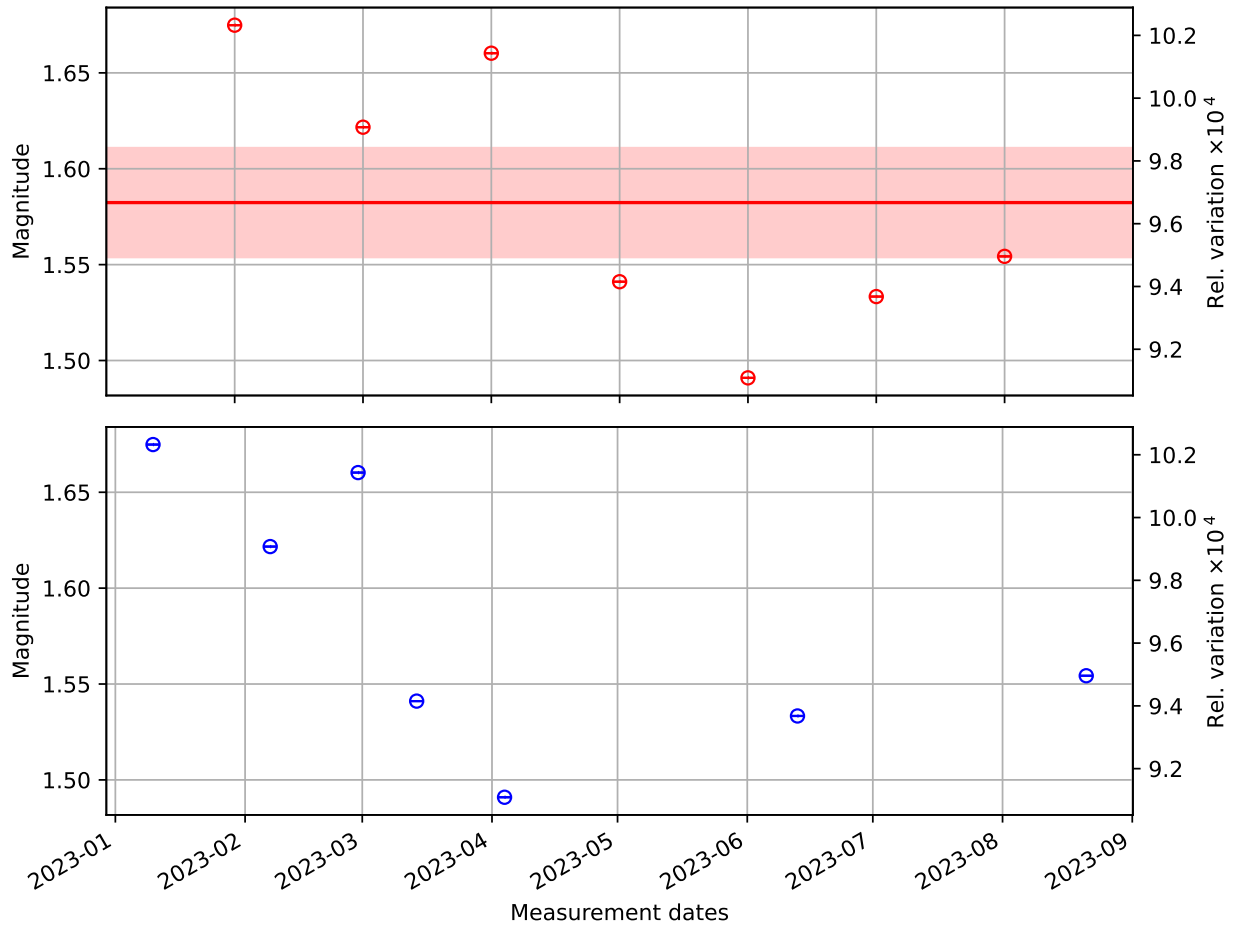


| Summary of ADC conversion factor discrepancy

13 TxPD calibration ($\rho_{Tx} = \rho_G \cdot \alpha_{WG} \cdot \alpha_{TW} \cdot \zeta$)

List of Measurements

Date	rhoTx $\pm$ SD_rhoTx
D20230110	8335.8363 $\pm$ 3.7737
D20230207	8331.5608 $\pm$ 3.5832
D20230228	8334.6371 $\pm$ 3.3555
D20230314	8333.3272 $\pm$ 3.4285
D20230404	8330.5796 $\pm$ 3.5576
D20230613	8323.3328 $\pm$ 3.1747
D20230821	8322.2378 $\pm$ 3.2788

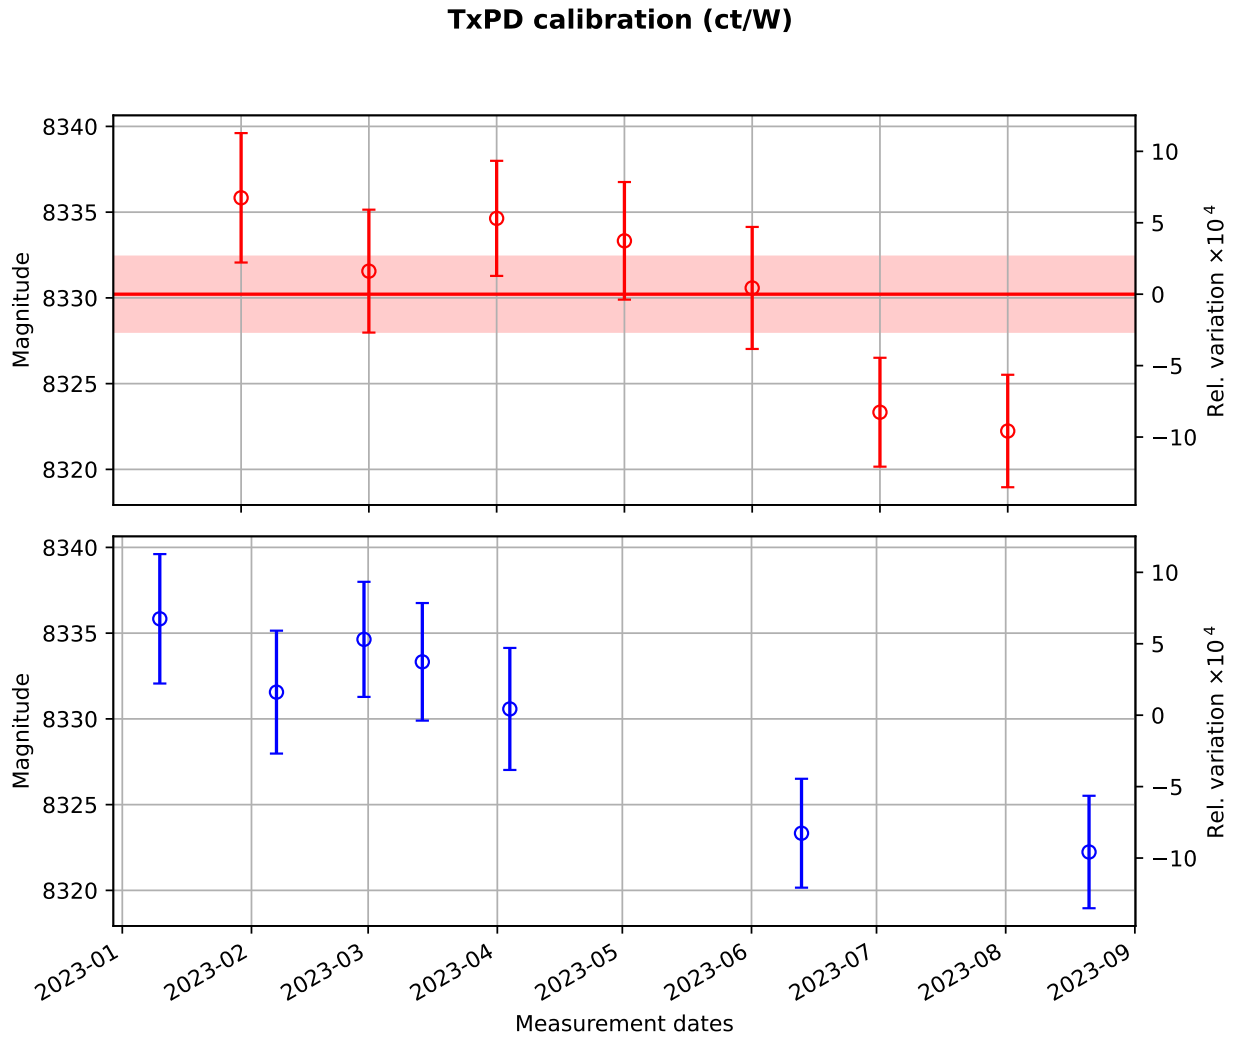


Summary of TxPD calibration (ct/W)		
Mean value:	8330.215937	
Standard deviation:	5.381839	
Standard error:	2.190190	
Relative Standard error:	0.000263	

14 RxPD calibration ($\rho_{Rx} = \rho_G \cdot \alpha_{WG} \cdot \alpha_{RW} \cdot \zeta$)

List of Measurements

Date	rhoRx $\pm$ SD_rhoRx
D20230110	10689.2786 $\pm$ 2.7664
D20230207	10682.9872 $\pm$ 3.1471
D20230228	10692.7178 $\pm$ 2.7391
D20230314	10695.3109 $\pm$ 2.6911
D20230404	10690.0120 $\pm$ 2.6817
D20230613	10676.0753 $\pm$ 2.8342
D20230821	10672.1188 $\pm$ 2.7358

RxPD calibration (ct/W)

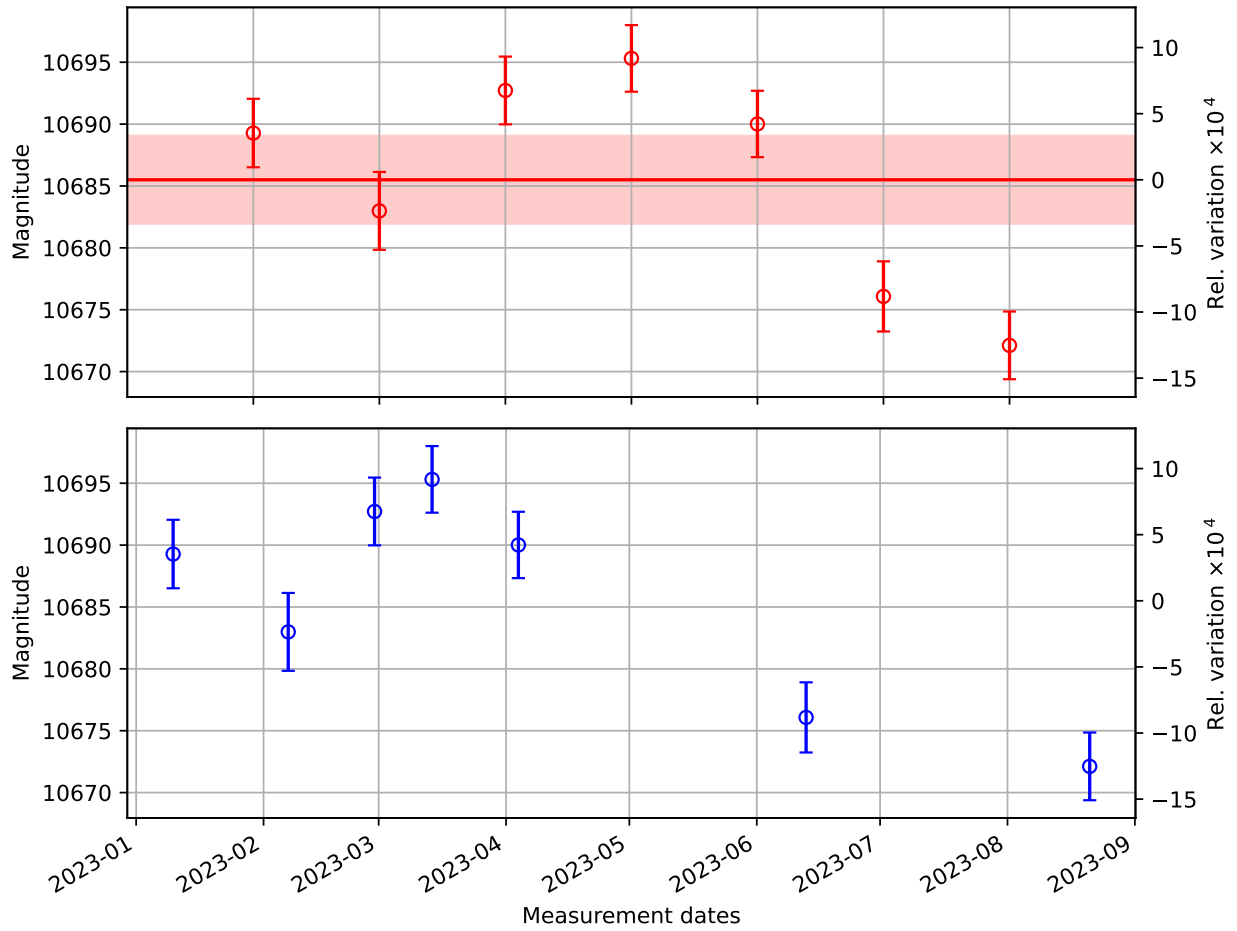

Summary of RxPD calibration (ct/W)


Mean value:	10685.500080
Standard deviation:	8.729082
Standard error:	3.552382
Relative Standard error:	0.000332

15 Optical Efficiency of Inner Beam $e^i = m3/m1$

List of Measurements

Date	$e_i \pm SD_{e_i}$
D20230110	0.9880 ± 0.0010
D20230207	0.9868 ± 0.0010
D20230228	0.9873 ± 0.0009
D20230314	0.9862 ± 0.0010
D20230404	0.9869 ± 0.0010
D20230613	0.9866 ± 0.0009
D20230821	0.9856 ± 0.0009

Optical Efficiency (Inner Beam)

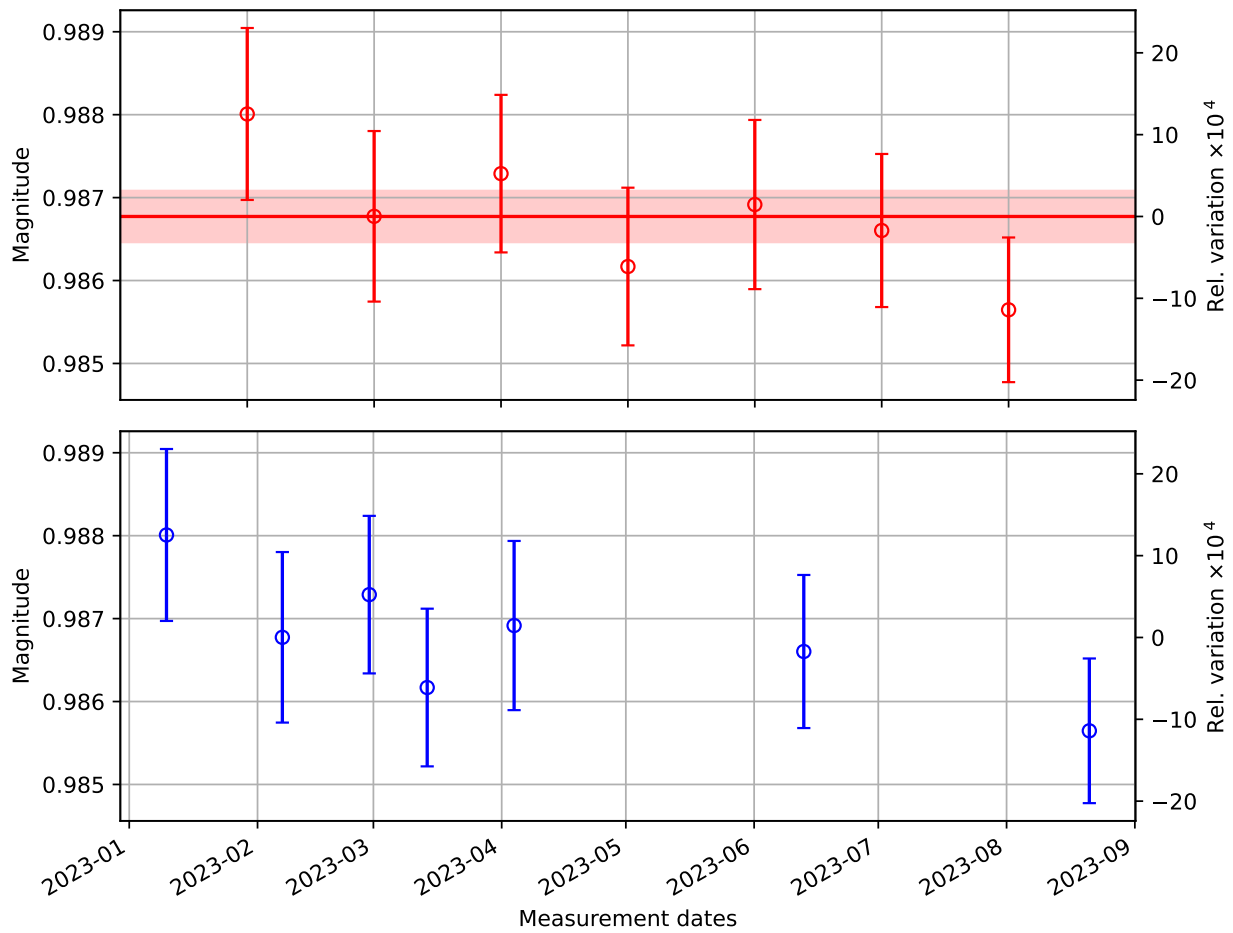

Summary of Optical Efficiency (Inner Beam)


Mean value:	0.986772
Standard deviation:	0.000761
Standard error:	0.000310
Relative Standard error:	0.000314

16 Optical Efficiency of Outer Beam $e^0 = m_4/m_2$

List of Measurements

Date	$e_o \pm SD_{e_o}$
D20230110	0.9877 ± 0.0010
D20230207	0.9877 ± 0.0010
D20230228	0.9895 ± 0.0009
D20230314	0.9887 ± 0.0009
D20230404	0.9894 ± 0.0009
D20230613	0.9850 ± 0.0009
D20230821	0.9862 ± 0.0010

Optical Efficiency (Outer Beam)

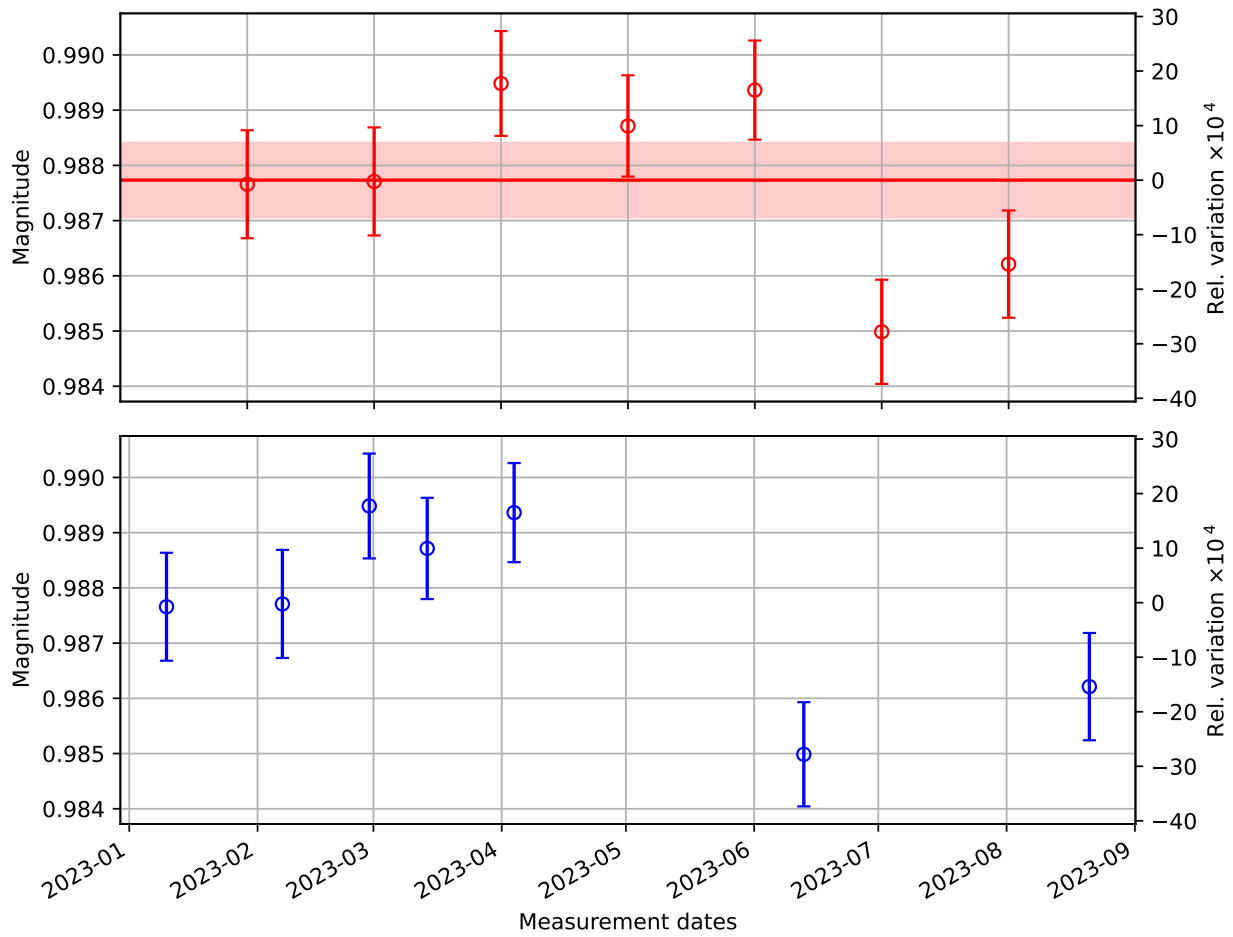

Summary of Optical Efficiency (Outer Beam)


Mean value:	0.987733
Standard deviation:	0.001661
Standard error:	0.000676
Relative Standard error:	0.000684

17 Total Optical Efficiency $e = (m3 + m4)/(m1 + m2)$

List of Measurements

Date	$e \pm SD_e$
D20230110	0.9878 ± 0.0007
D20230207	0.9872 ± 0.0007
D20230228	0.9884 ± 0.0007
D20230314	0.9875 ± 0.0007
D20230404	0.9881 ± 0.0007
D20230613	0.9858 ± 0.0007
D20230821	0.9859 ± 0.0006

Overall Optical Efficiency

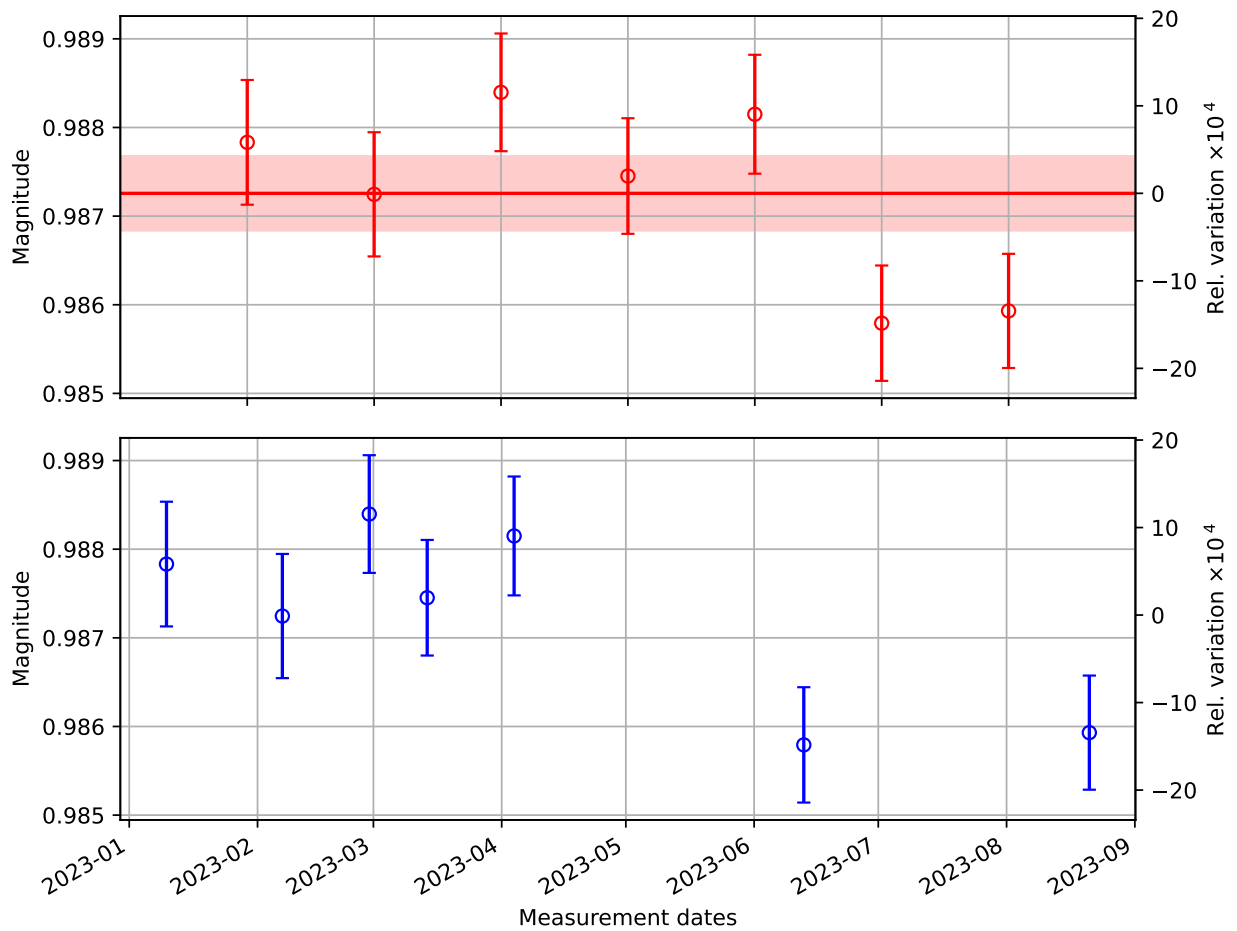


Summary of Overall Optical Efficiency

Mean value:	0.987257
Standard deviation:	0.001030
Standard error:	0.000419
Relative Standard error:	0.000425

18 Input/Output optical efficiency ratio (β)

List of Measurements

Date	beta $\pm$ SD_beta
D20230110	9.9889e-01 $\pm$ 1.0000e-09
D20230207	9.9889e-01 $\pm$ 1.0000e-09
D20230228	9.9889e-01 $\pm$ 1.0000e-09
D20230314	9.9889e-01 $\pm$ 1.0000e-09
D20230404	9.9889e-01 $\pm$ 1.0000e-09
D20230613	9.9889e-01 $\pm$ 1.0000e-09
D20230821	9.9889e-01 $\pm$ 1.0000e-09

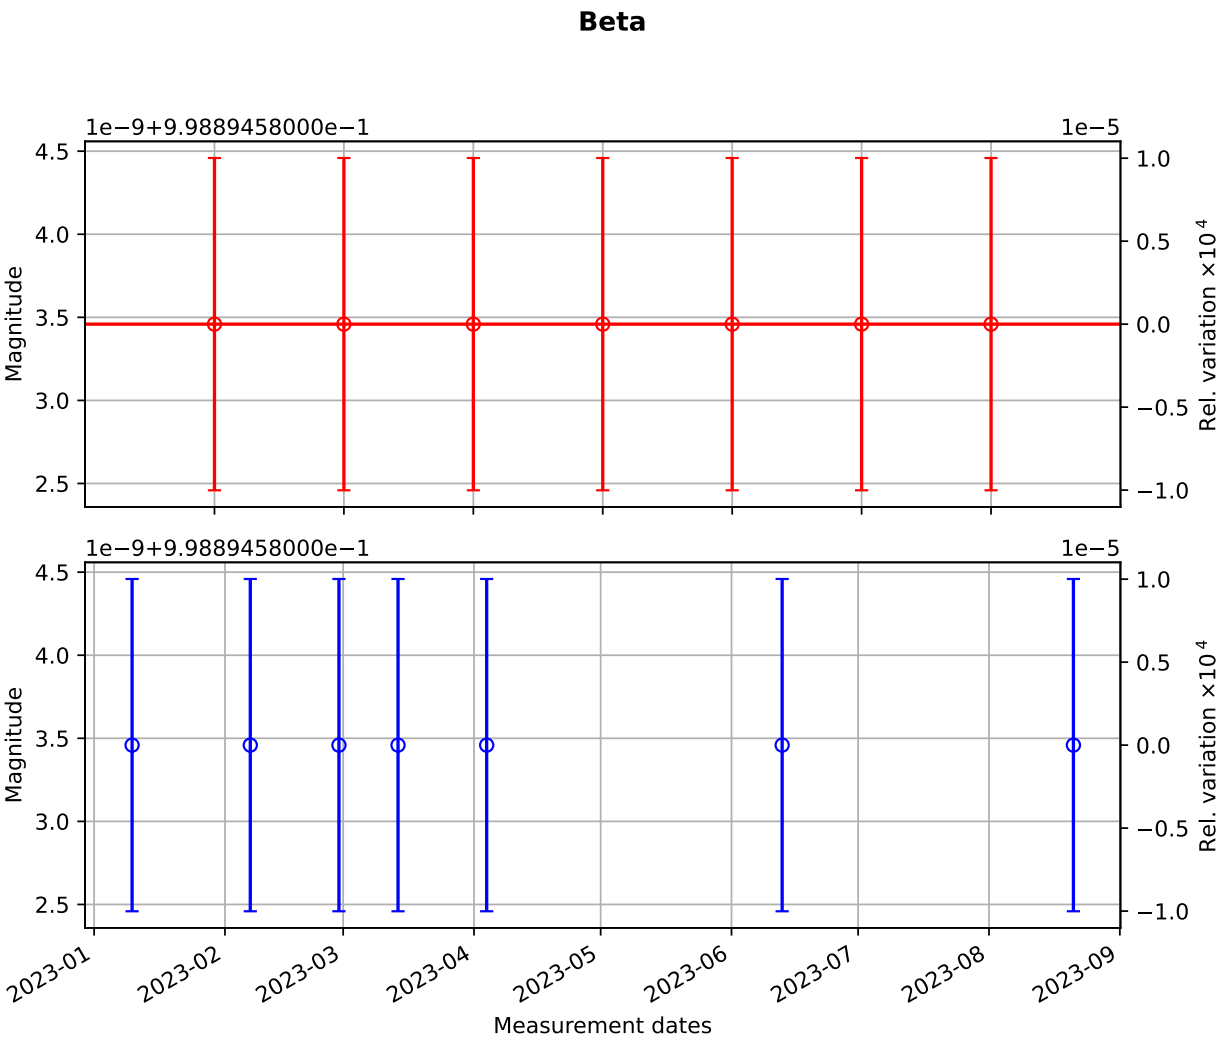


Summary of Beta		
Mean value:	0.998895	
Standard deviation:	0.000000	
Standard error:	0.000000	
Relative Standard error:	0.000000	

19 Input Optical efficiency correction factor ($\eta_T = \sqrt{e \cdot \beta}$)

List of Measurements

Date	E_T $\pm$ SD_E_T
D20230110	0.9933 $\pm$ 0.0007
D20230207	0.9931 $\pm$ 0.0007
D20230228	0.9936 $\pm$ 0.0007
D20230314	0.9932 $\pm$ 0.0007
D20230404	0.9935 $\pm$ 0.0007
D20230613	0.9923 $\pm$ 0.0007
D20230821	0.9924 $\pm$ 0.0006

Input Side Optical Efficiency correction factor

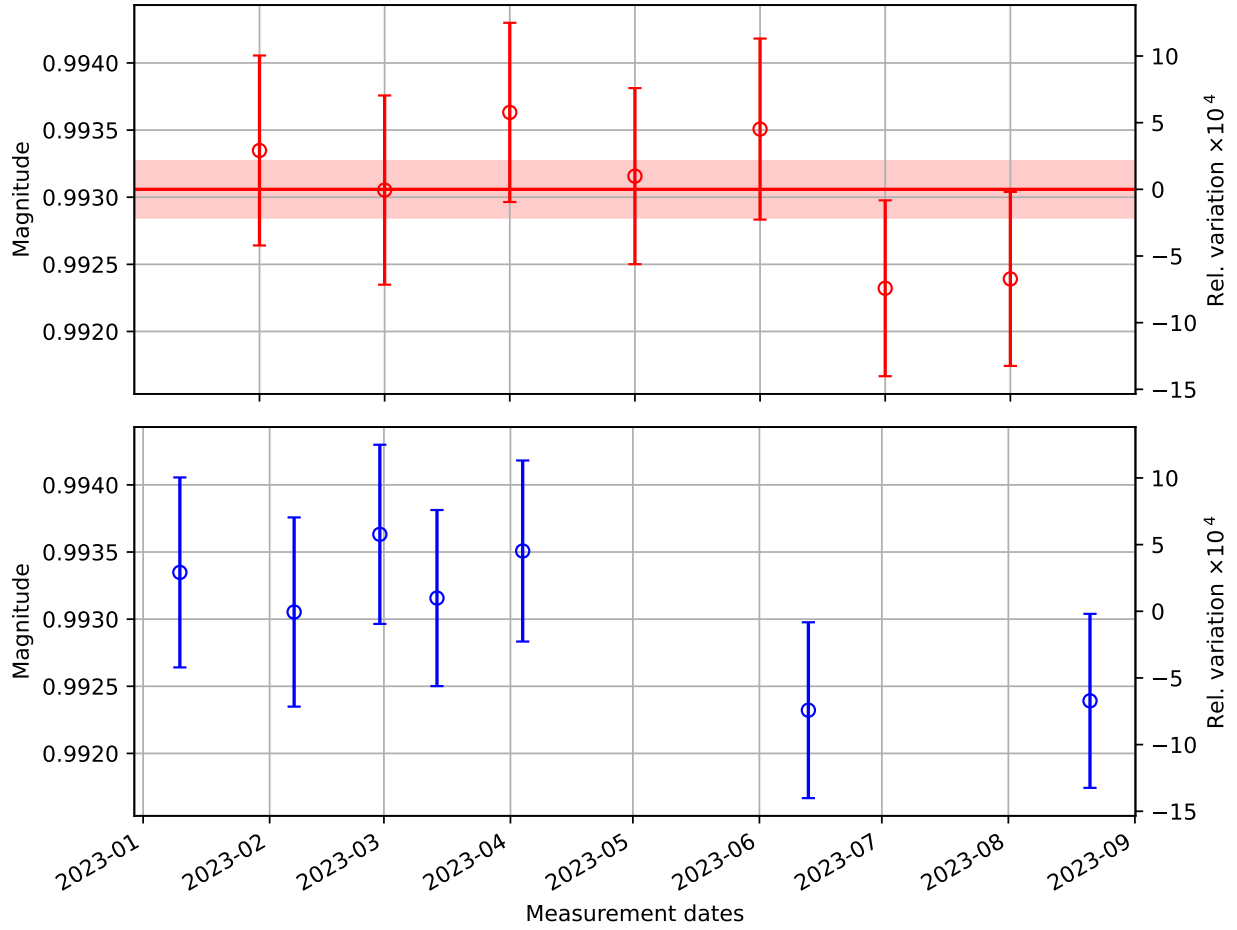


Summary of Input Side Optical Efficiency correction factor		
Mean value:	0.993059	
Standard deviation:	0.000518	
Standard error:	0.000211	
Relative Standard error:	0.000212	

20 Output Optical efficiency correction factor ($\eta_R = \sqrt{e/\beta}$)

List of Measurements

Date	E_R $\pm$ SD_E_R
D20230110	0.9944 $\pm$ 0.0007
D20230207	0.9942 $\pm$ 0.0007
D20230228	0.9947 $\pm$ 0.0007
D20230314	0.9943 $\pm$ 0.0007
D20230404	0.9946 $\pm$ 0.0007
D20230613	0.9934 $\pm$ 0.0007
D20230821	0.9935 $\pm$ 0.0006

Output Side Optical Efficiency correction factor

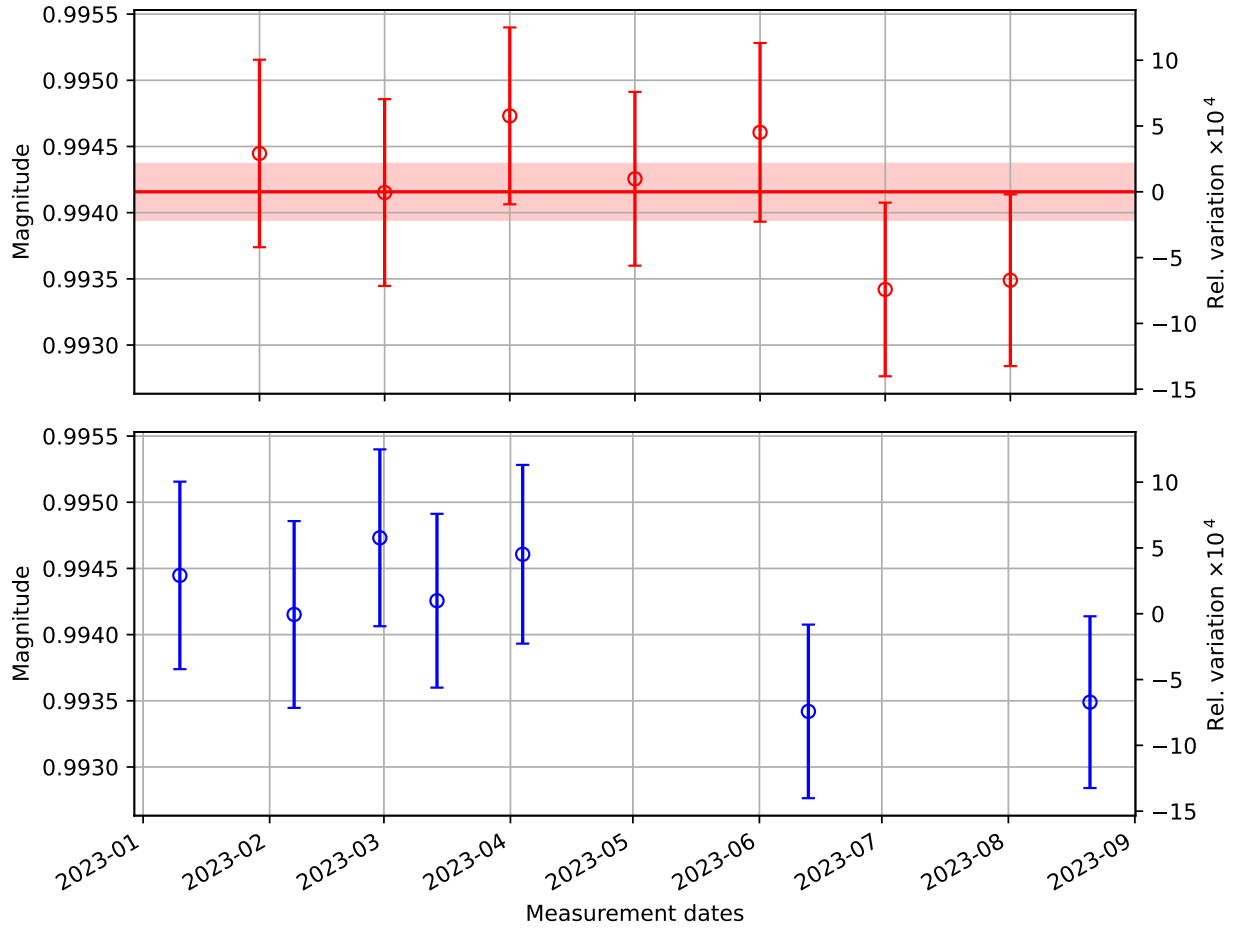

Summary of Output Side Optical Efficiency correction factor


Mean value:	0.994158
Standard deviation:	0.000519
Standard error:	0.000211
Relative Standard error:	0.000212

21 TxPD calibration at ETM ($\rho'_{Tx} = \rho_T \cdot \eta_T \cdot \zeta$)

List of Measurements

Date	rhoT_prime $\pm$ SD_rhoT_prime
D20230110	8391.6574 $\pm$ 7.0818
D20230207	8389.8439 $\pm$ 6.9612
D20230228	8388.0549 $\pm$ 6.5683
D20230314	8390.7454 $\pm$ 6.5279
D20230404	8385.0193 $\pm$ 6.7238
D20230613	8387.7359 $\pm$ 6.3941
D20230821	8386.0437 $\pm$ 6.3956

TxPD calibration corrected for optical efficiency (ct/W)

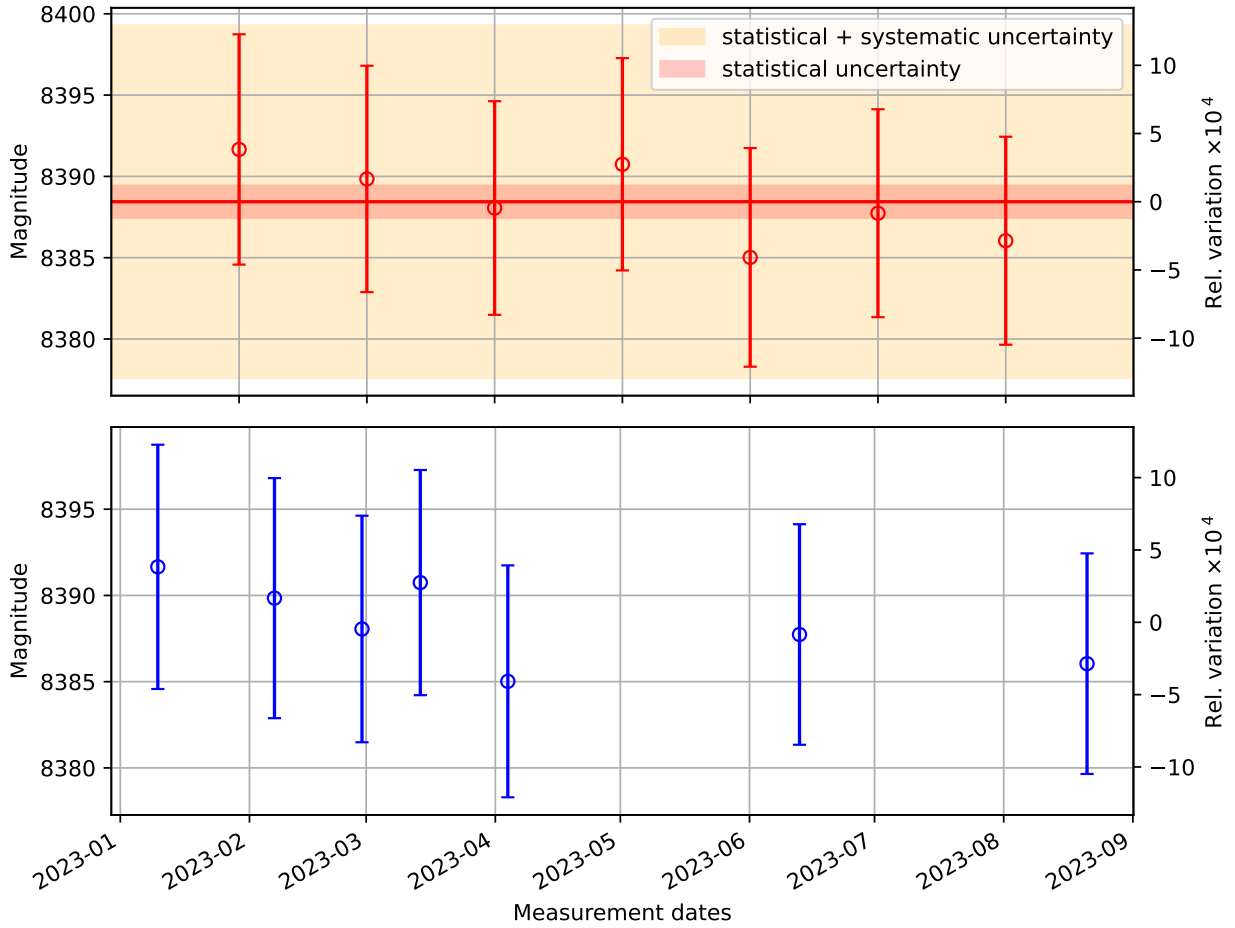


Summary of TxPD calibration corrected for optical efficiency (ct/W)	
Mean value:	8388.442919
Standard deviation:	2.440125
Standard error:	0.993032
Relative Standard error:	0.000118

22 RxPD calibration at ETM ($\rho'_{Rx} = \rho_R \cdot \eta_R \cdot \zeta$)

List of Measurements

Date	rhoR_prime $\pm$ SD_rhoR_prime
D20230110	10629.9242 $\pm$ 8.0551
D20230207	10620.5139 $\pm$ 8.1595
D20230228	10636.3809 $\pm$ 7.6456
D20230314	10633.8774 $\pm$ 7.5141
D20230404	10632.3603 $\pm$ 7.6934
D20230613	10605.8257 $\pm$ 7.5452
D20230821	10602.6395 $\pm$ 7.4380

RxPD calibration corrected for optical efficiency (ct/W)

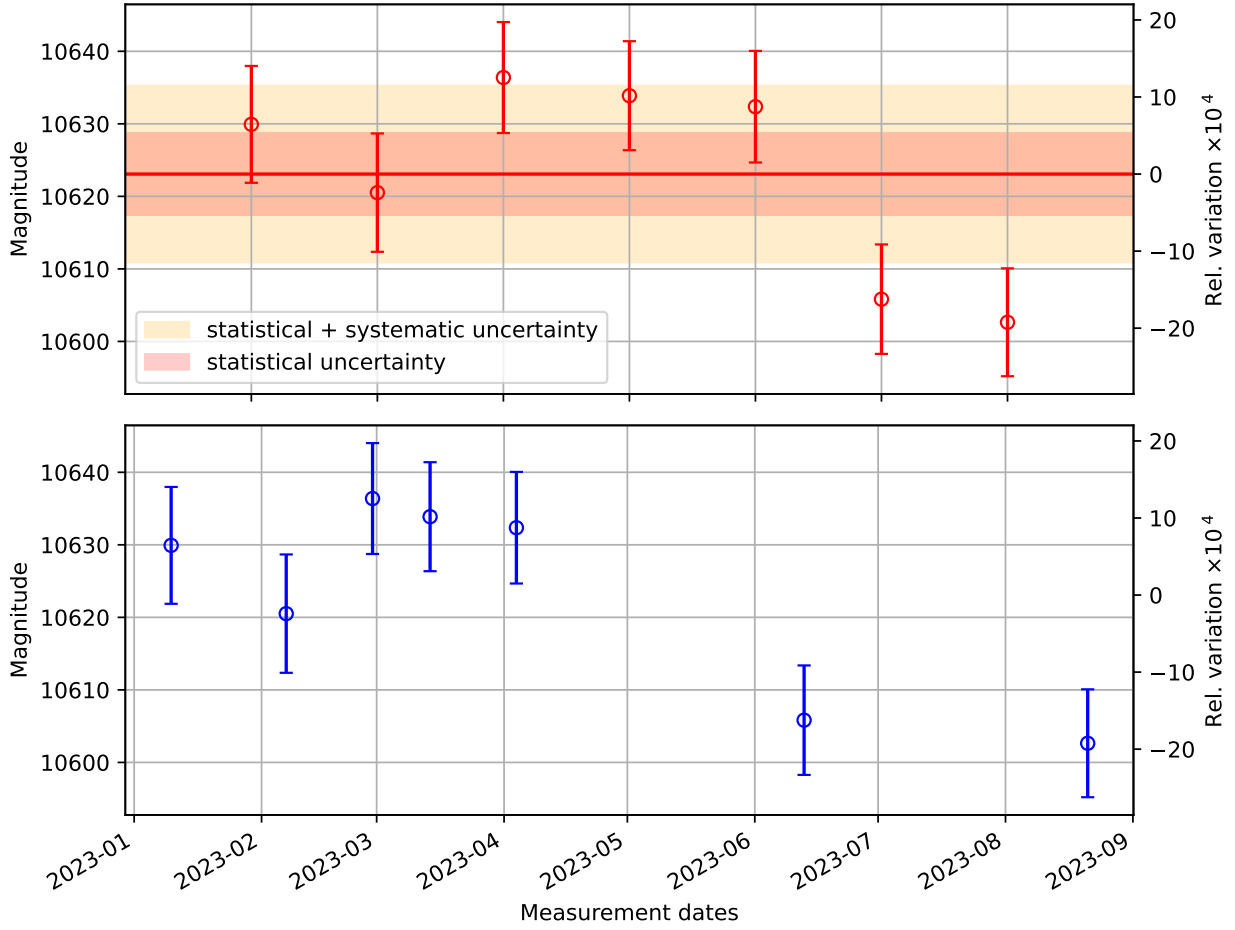


Summary of RxPD calibration corrected for optical efficiency (ct/W)	
Mean value:	10623.074549
Standard deviation:	13.835806
Standard error:	5.630611
Relative Standard error:	0.000530

23 Power Imbalance

List of Measurements

Date	PI $\pm$ SD_PI
D20230110	0.9849 $\pm$ 0.0011
D20230207	0.9832 $\pm$ 0.0010
D20230228	0.9814 $\pm$ 0.0009
D20230314	0.9834 $\pm$ 0.0009
D20230404	0.9843 $\pm$ 0.0010
D20230613	0.9936 $\pm$ 0.0009
D20230821	0.9924 $\pm$ 0.0009

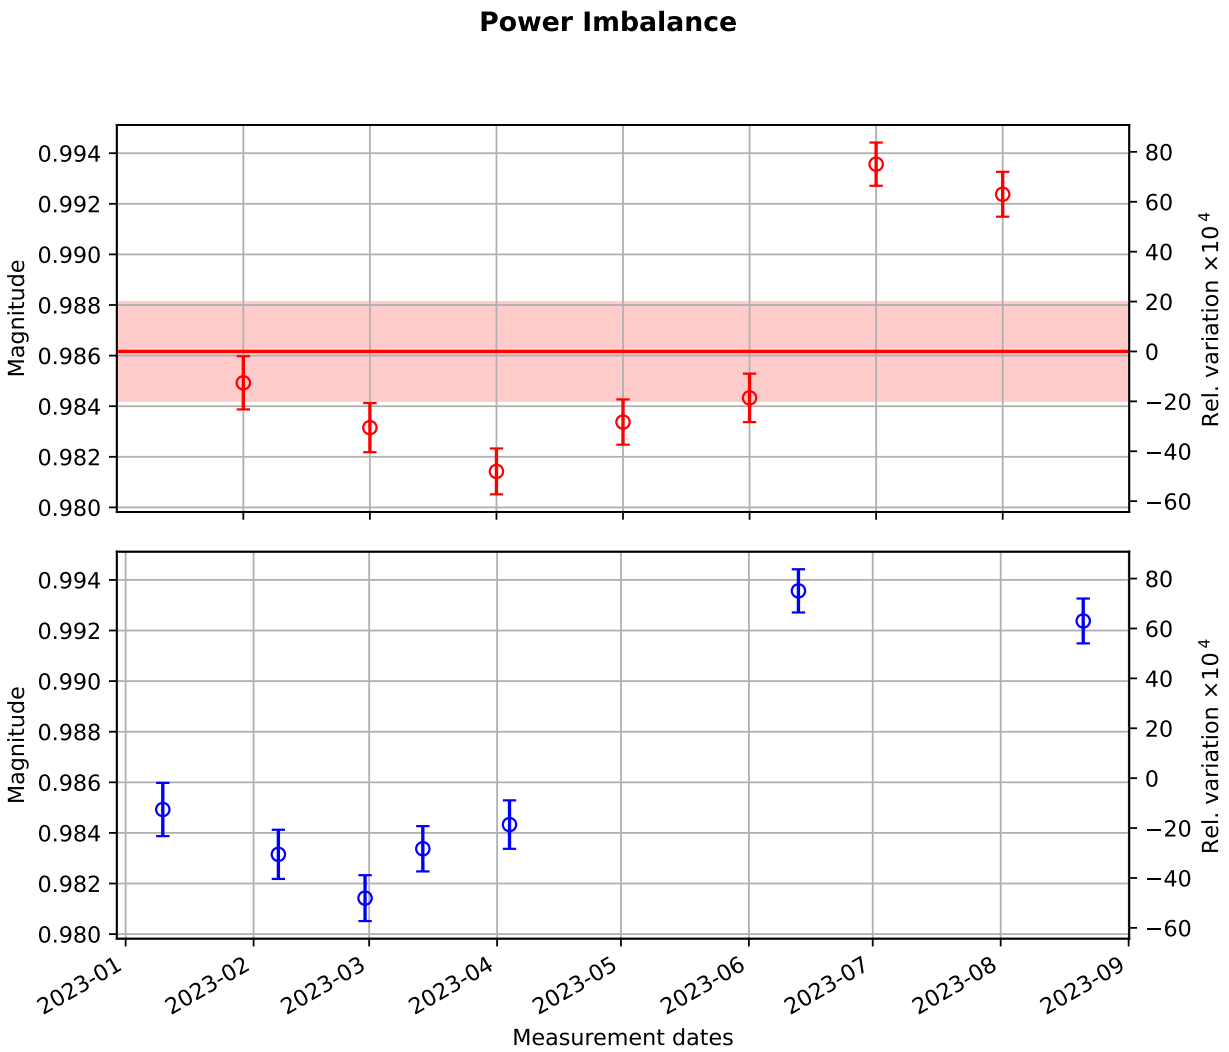

Summary of Power Imbalance		
Mean value:	0.986164	
Standard deviation:	0.004790	
Standard error:	0.001949	
Relative Standard error:	0.001977	