



Coupling at MC-tube from HVAC-scale vibration

Noise is produced even off-resonance

DARM



Accelerometer

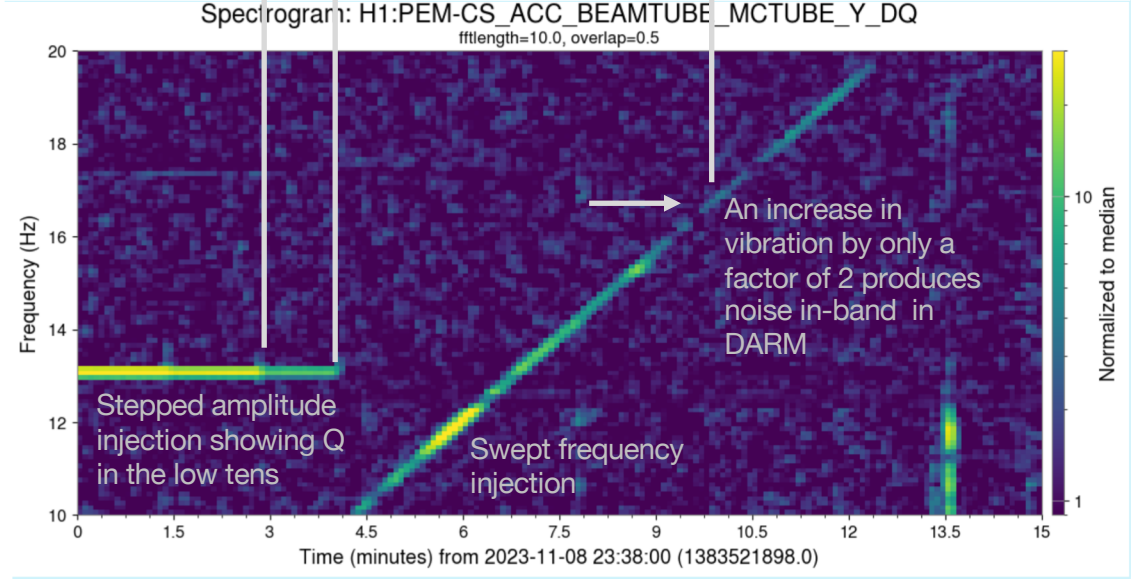

Below: An injection that is roughly consistent with the HVAC increase produces noise in DARM.

Spectra from the MC-tube accelerometer. Red: nominal, Blue: all CS HVAC turbines off. Black: part of the sweep shown in the spectrogram with an arrow pointing to the shaking peak at the point indicted in the spectrogram.

