


P\_AS vs P\_DCPD 430 kW, 18 hr lock, ETMX RH 1.3, ETMY RH 1.2

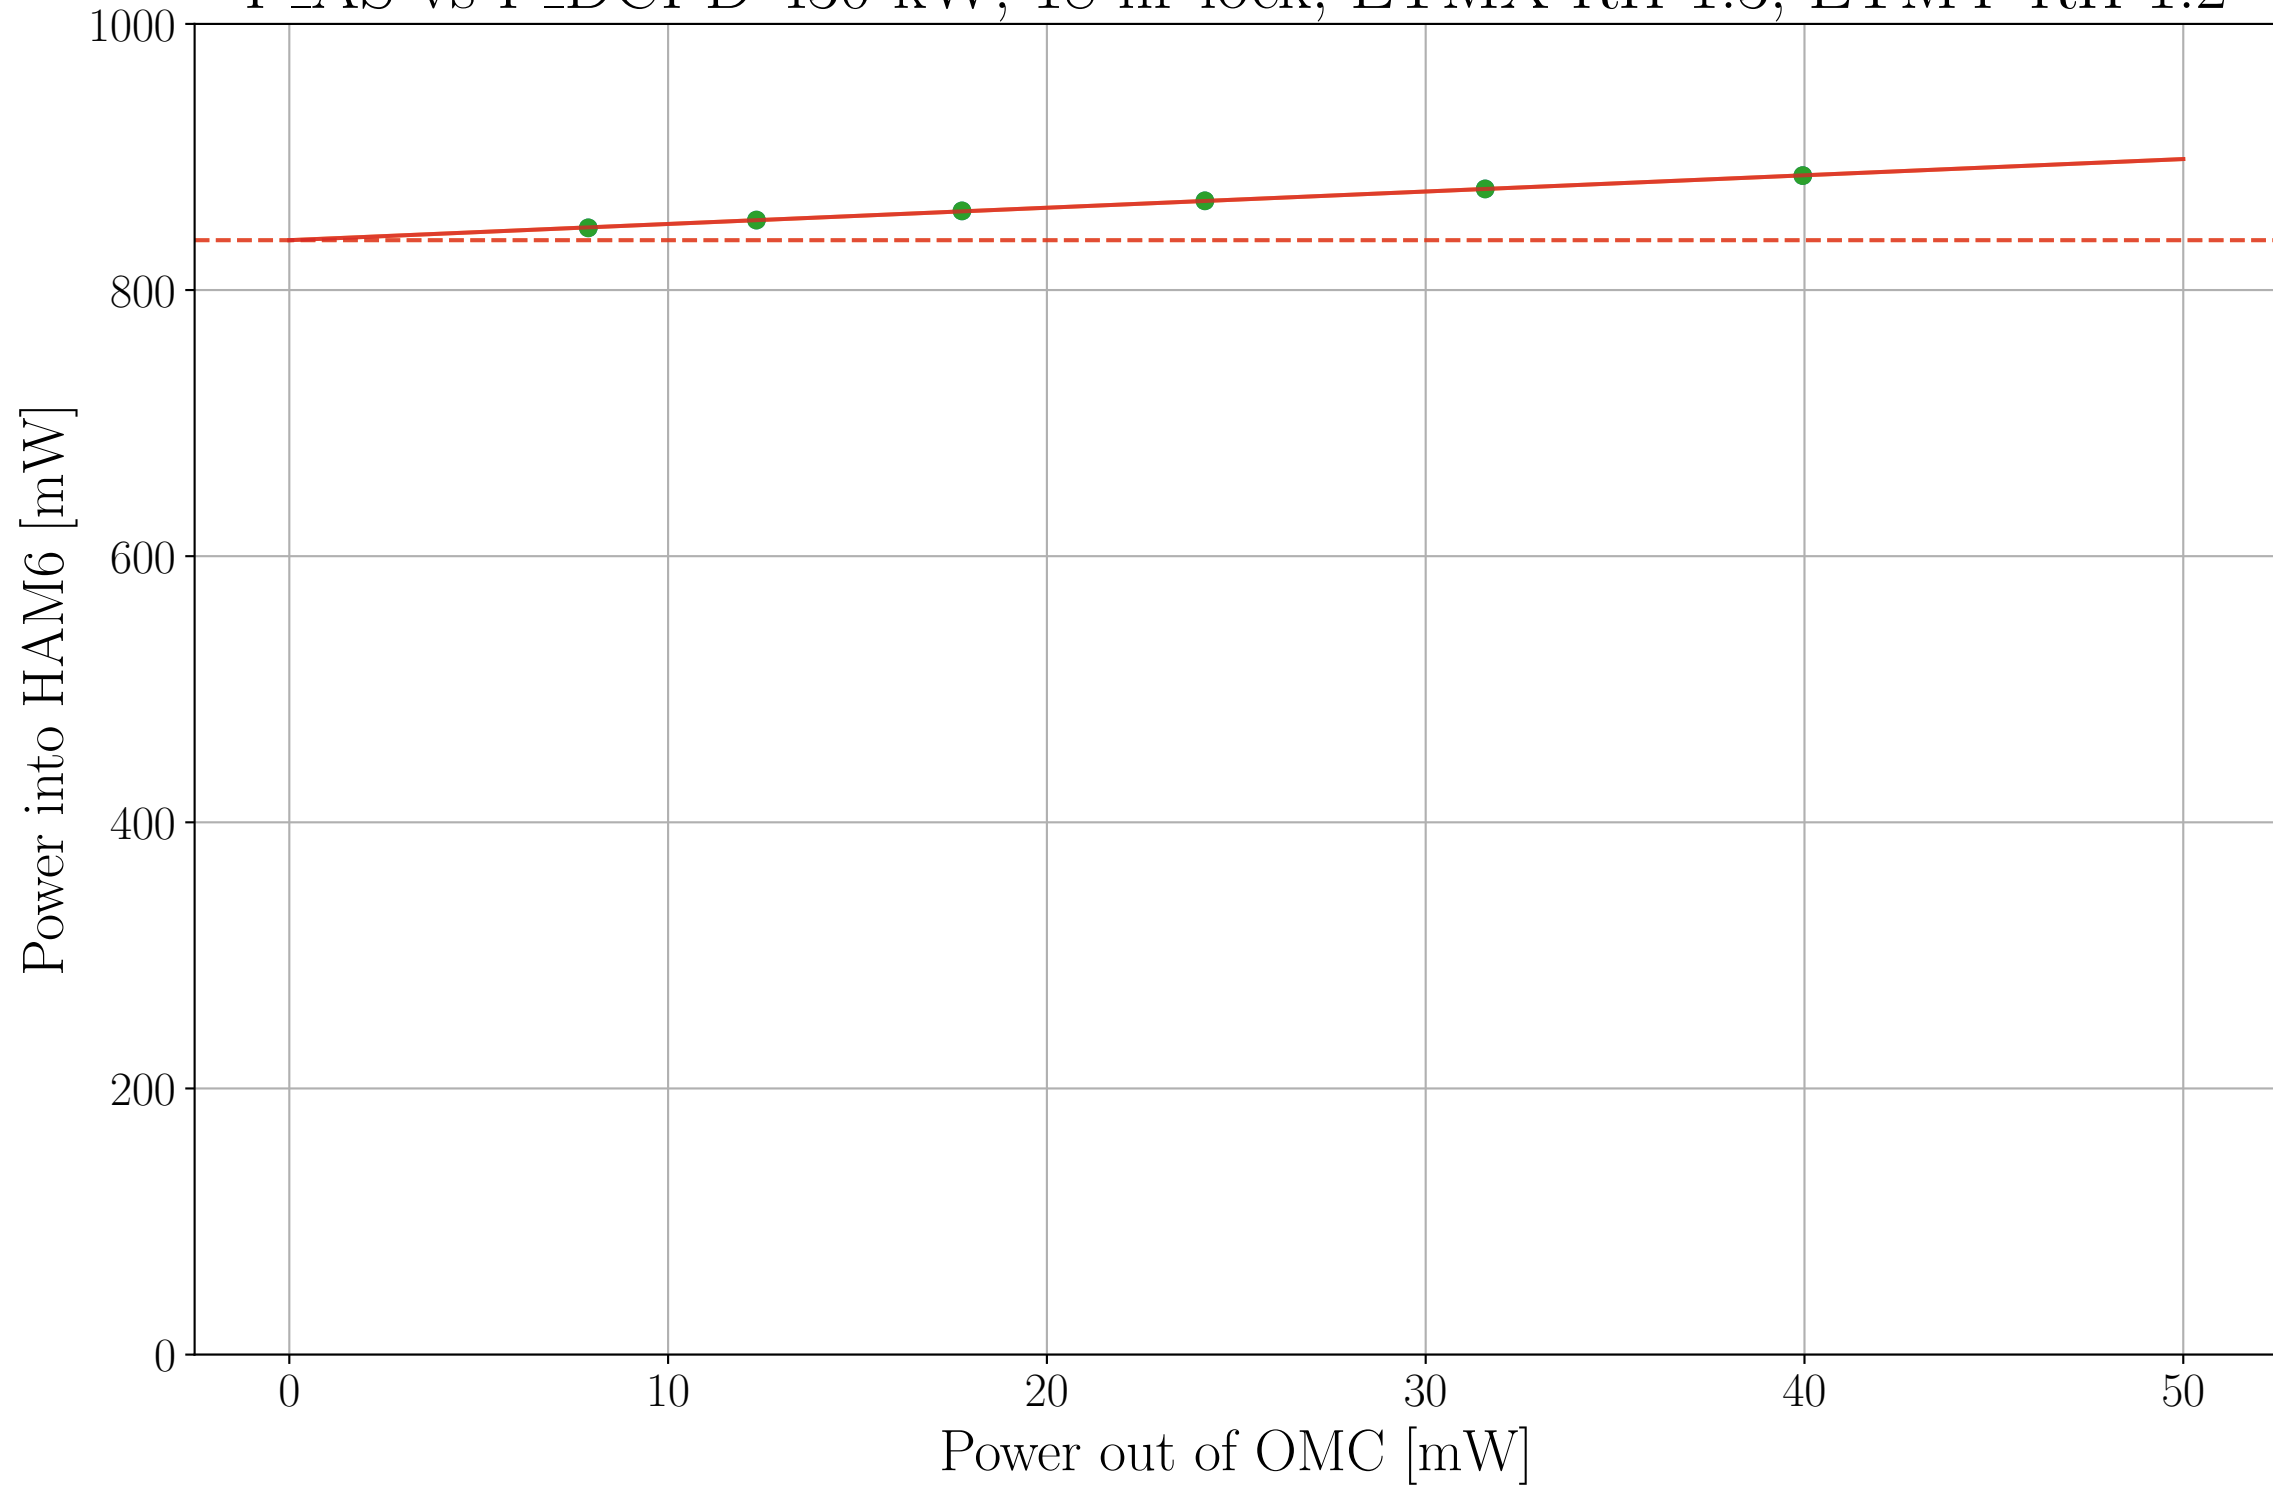

- Data at 255.0 Hz  
Linear fit  $ax + b$   
Slope  $a$  [mW/mW] =  $1.219 \pm 0.010$   
Intercept  $b$  [mW] =  $837.467 \pm 0.255$
- P\_as which is insensitive to DARM = 837.467 mW
- Data at 410.3 Hz  
Linear fit  $ax + b$   
Slope  $a$  [mW/mW] =  $1.219 \pm 0.010$   
Intercept  $b$  [mW] =  $837.467 \pm 0.255$
- - - P\_as which is insensitive to DARM = 837.467 mW